

FIG. 2

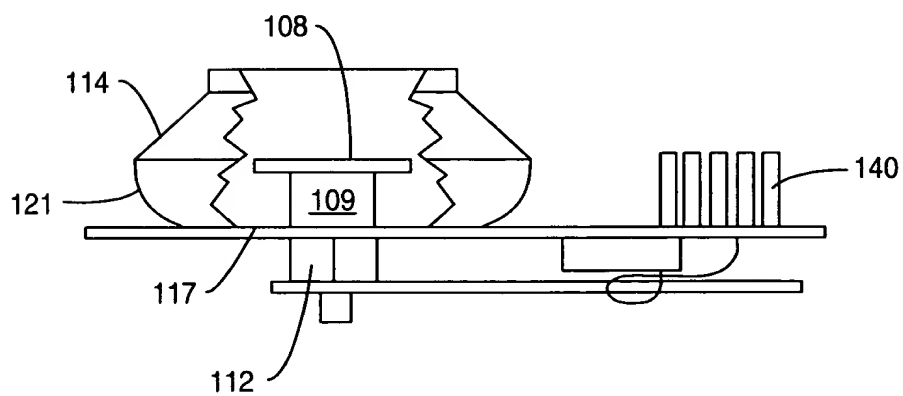


FIG. 3

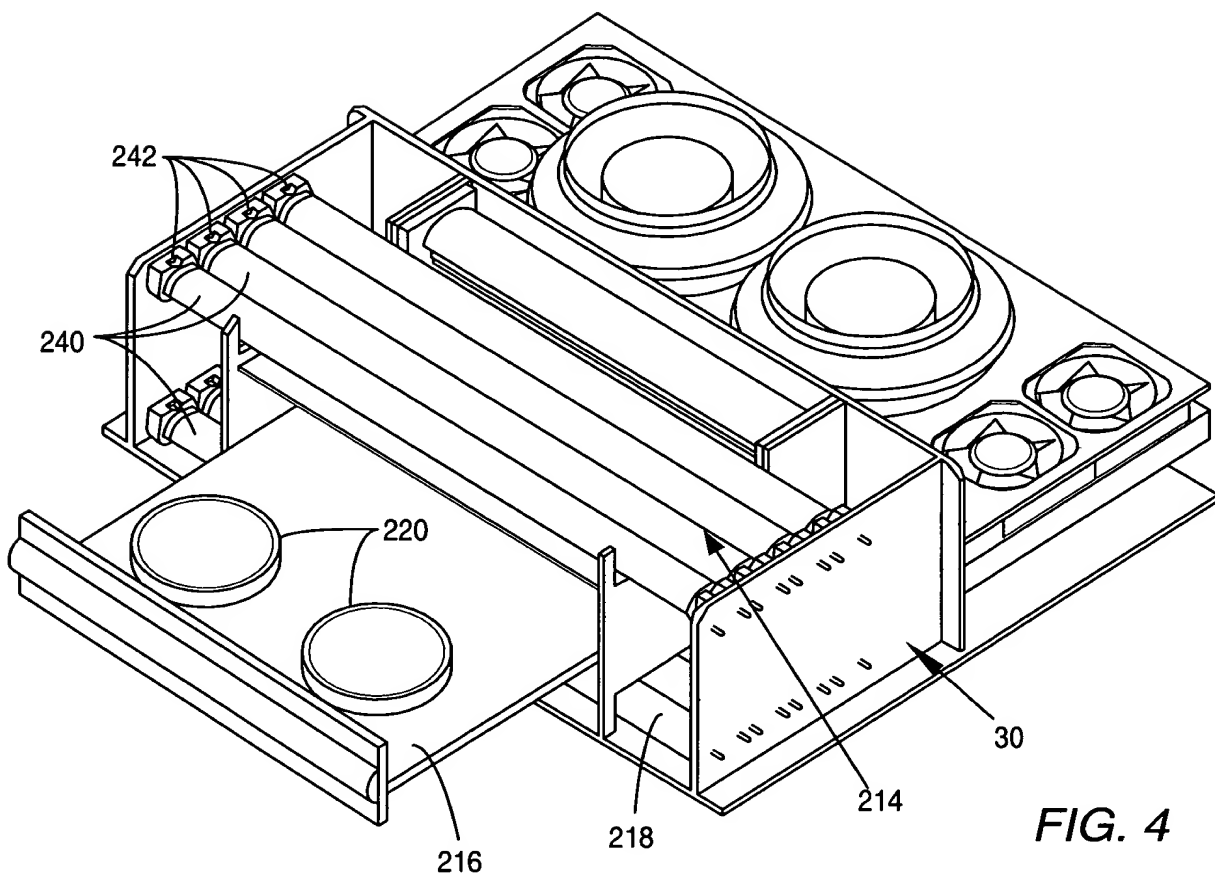


FIG. 4

4/42

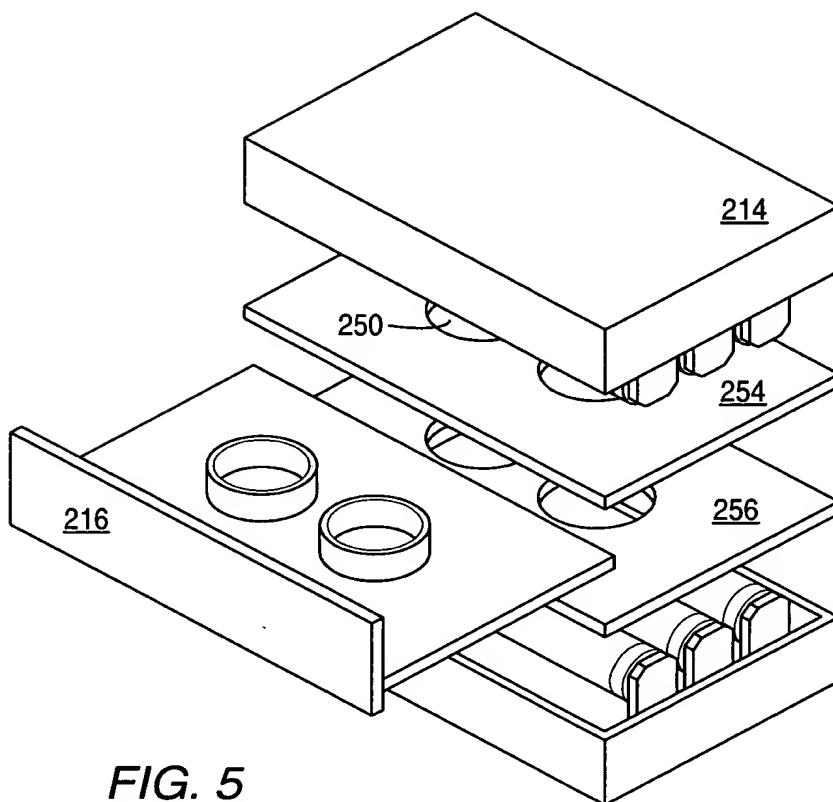


FIG. 5

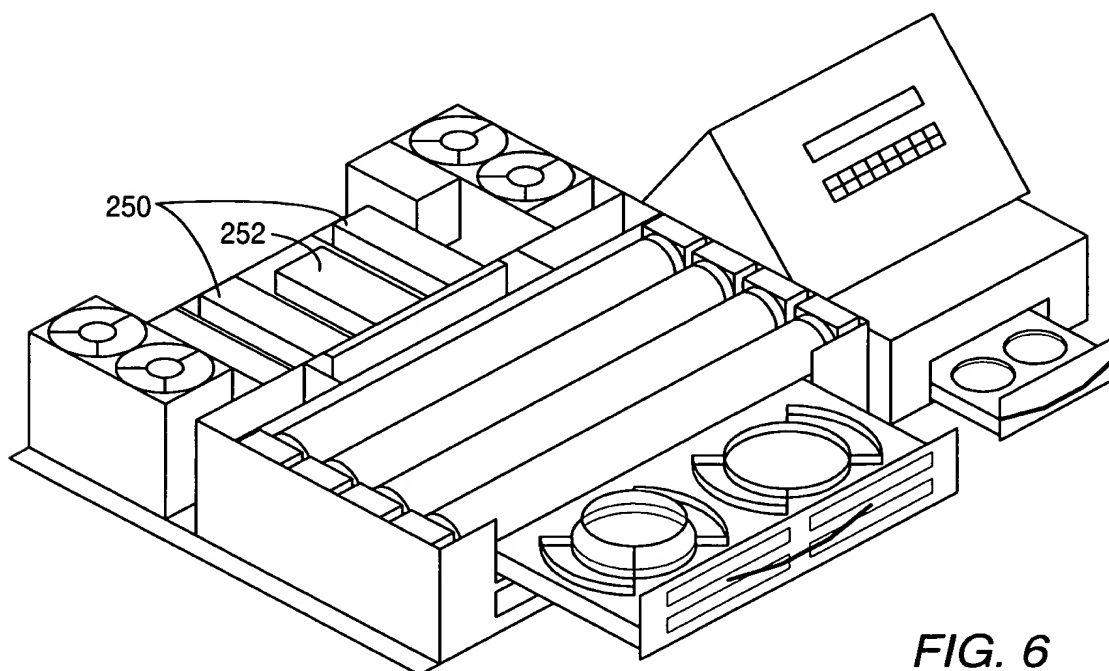


FIG. 6

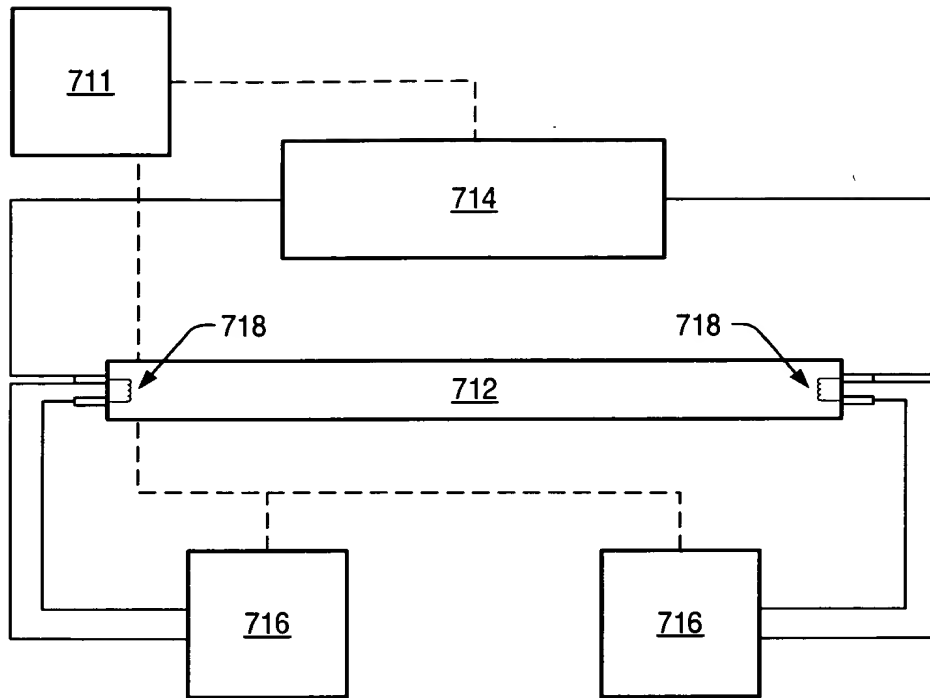


FIG. 7

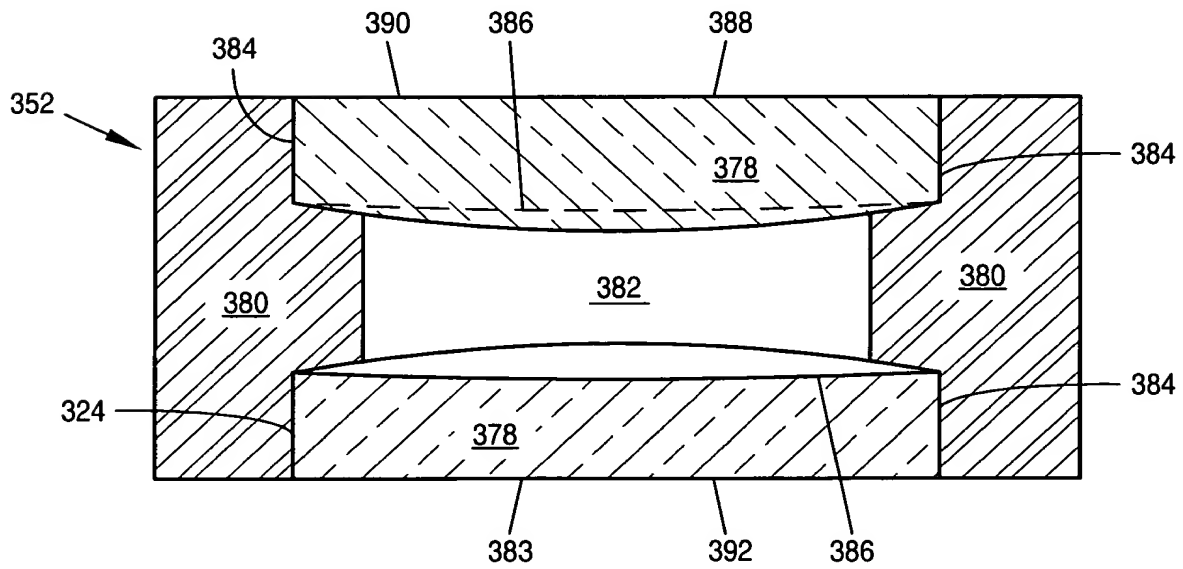
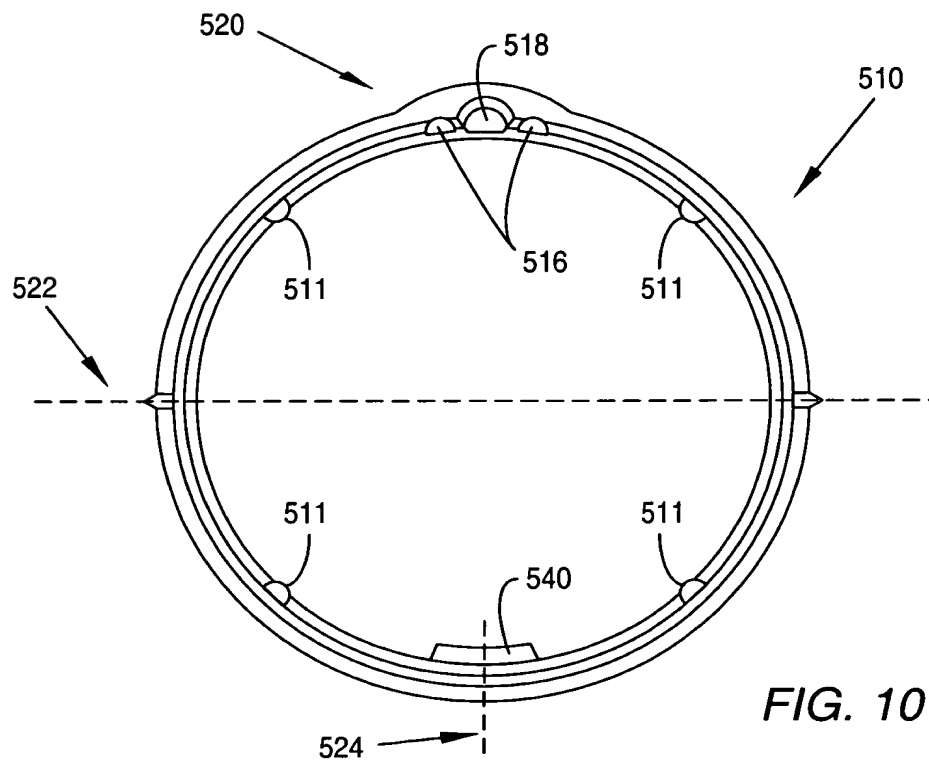
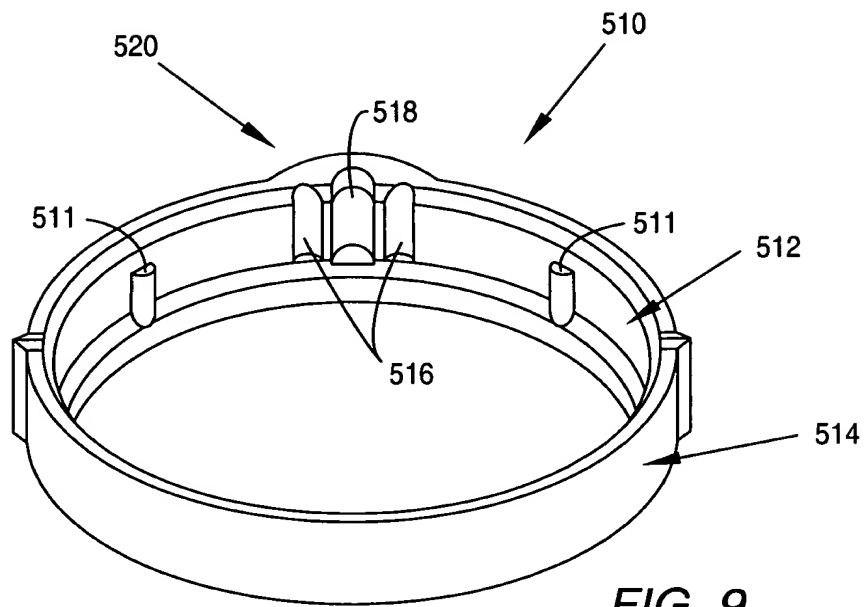


FIG. 8

6/42



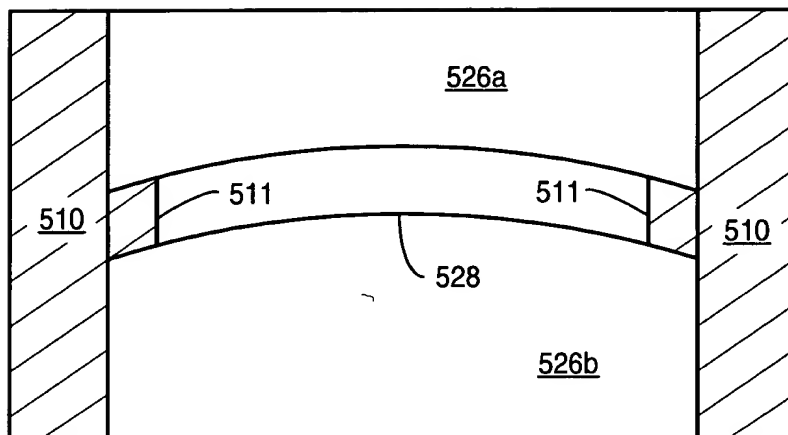


FIG. 11

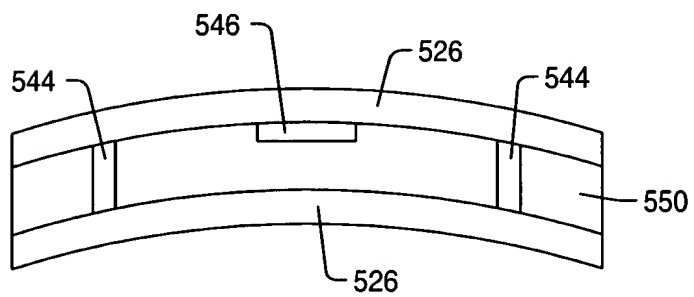


FIG. 14

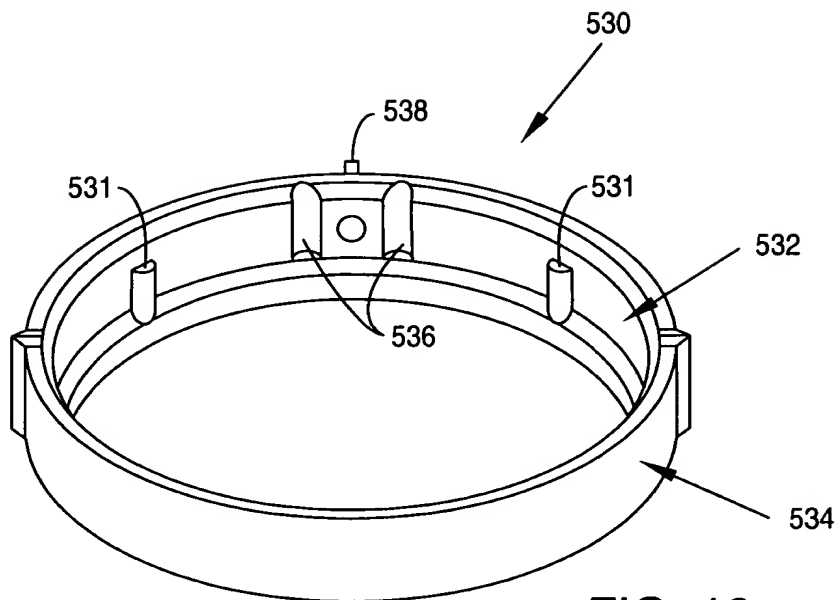


FIG. 12

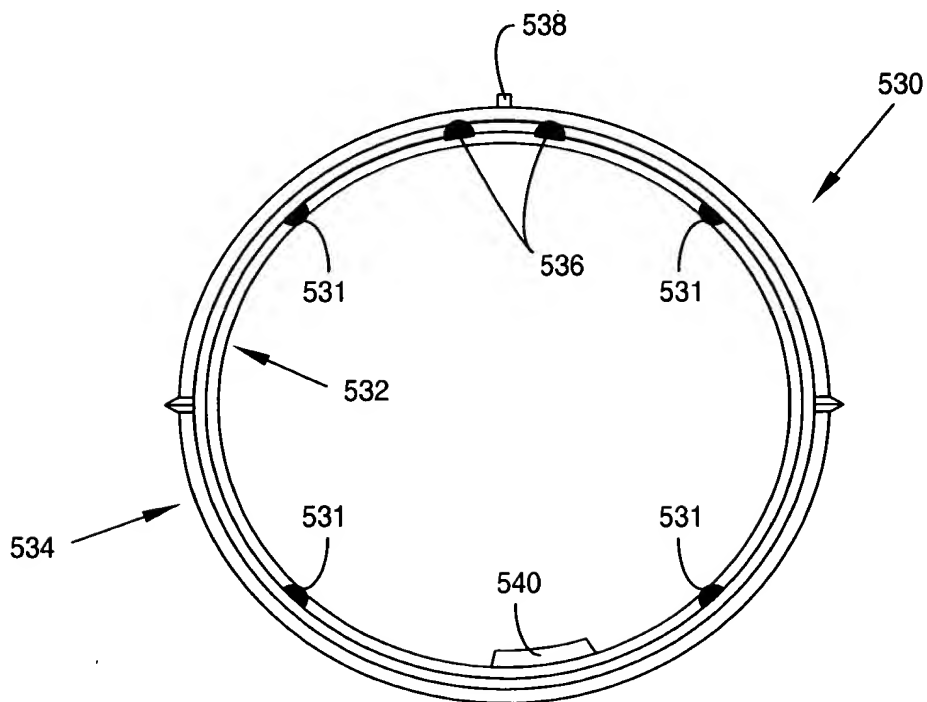


FIG. 13

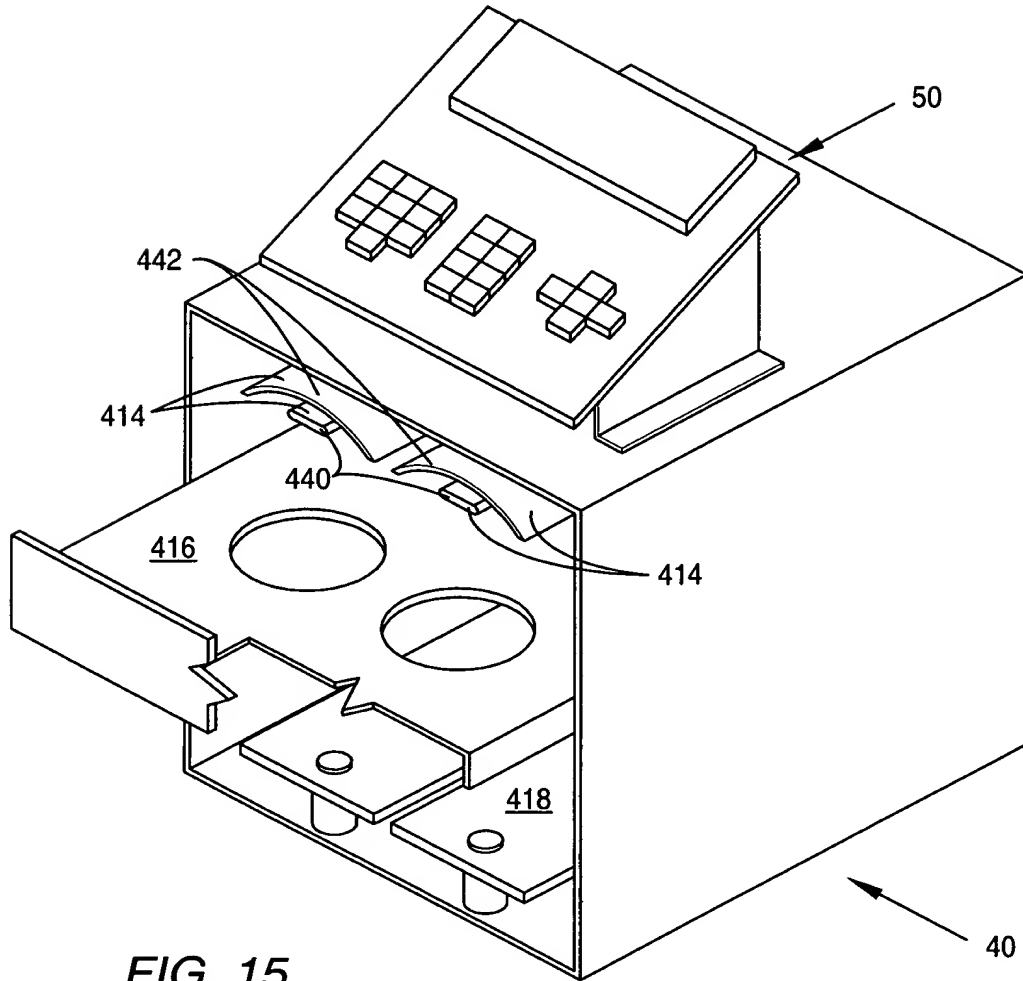


FIG. 15

10/42

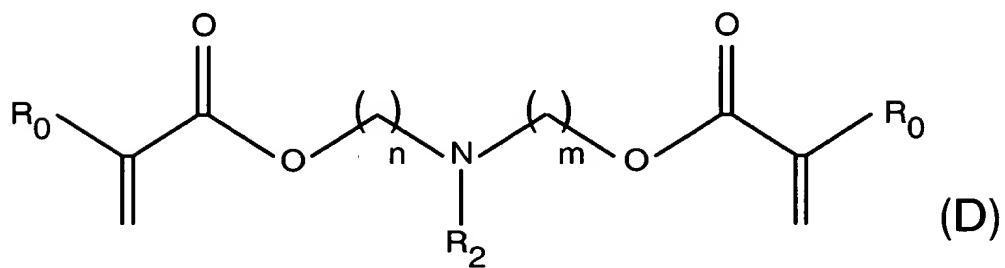
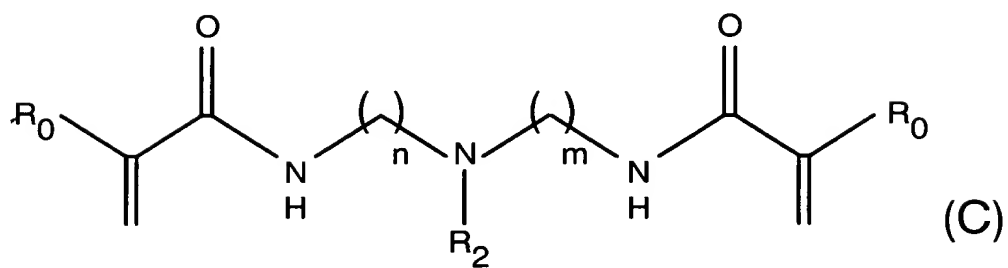
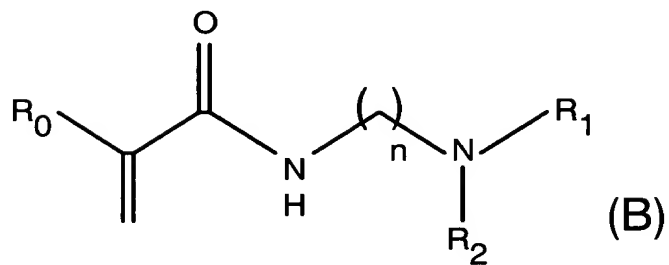
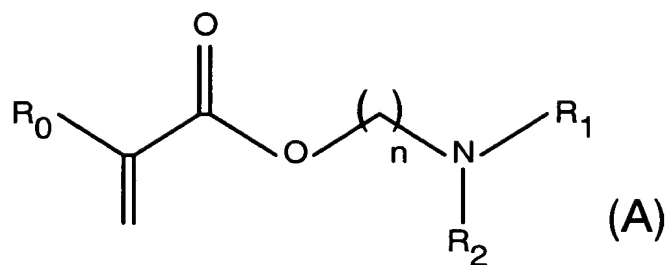


FIG. 16

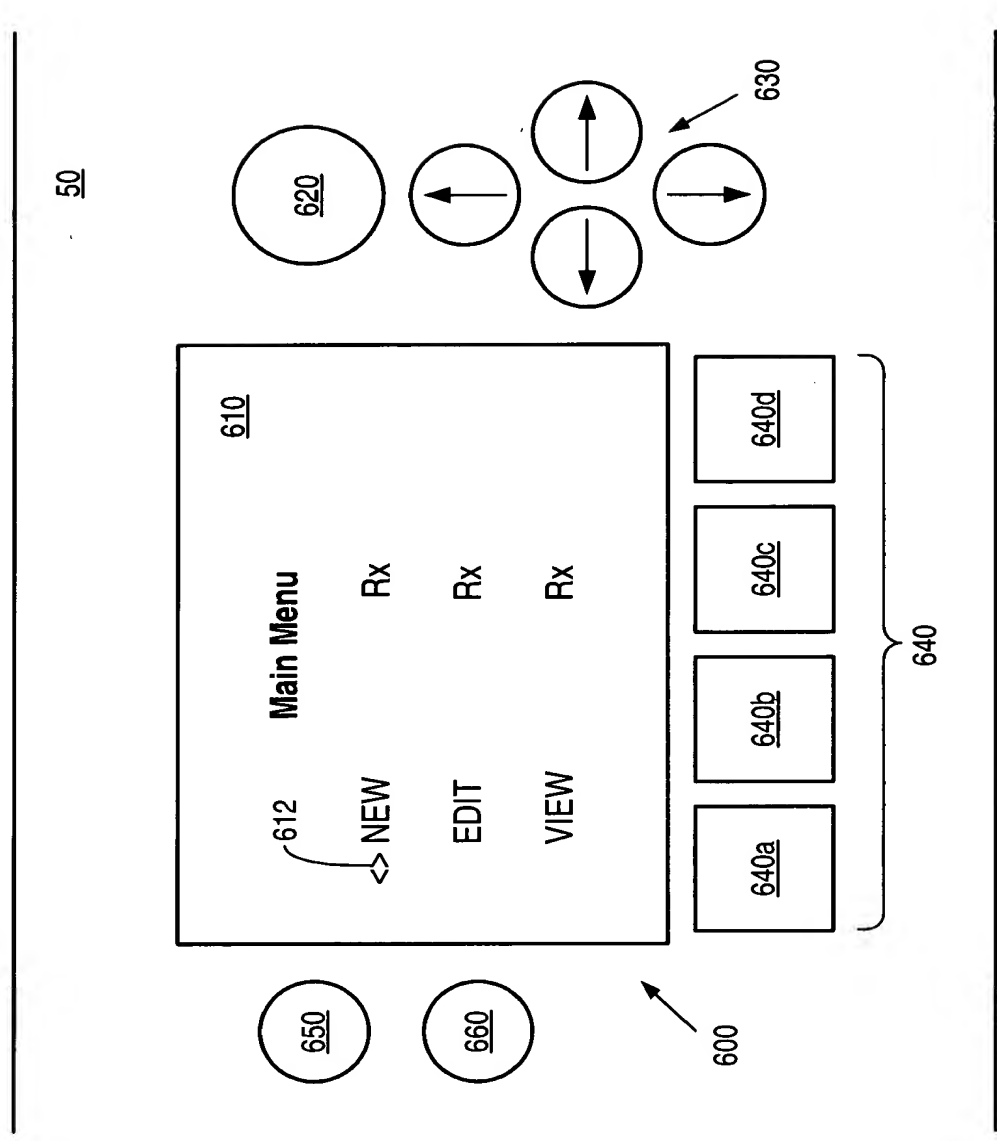


FIG. 17

50

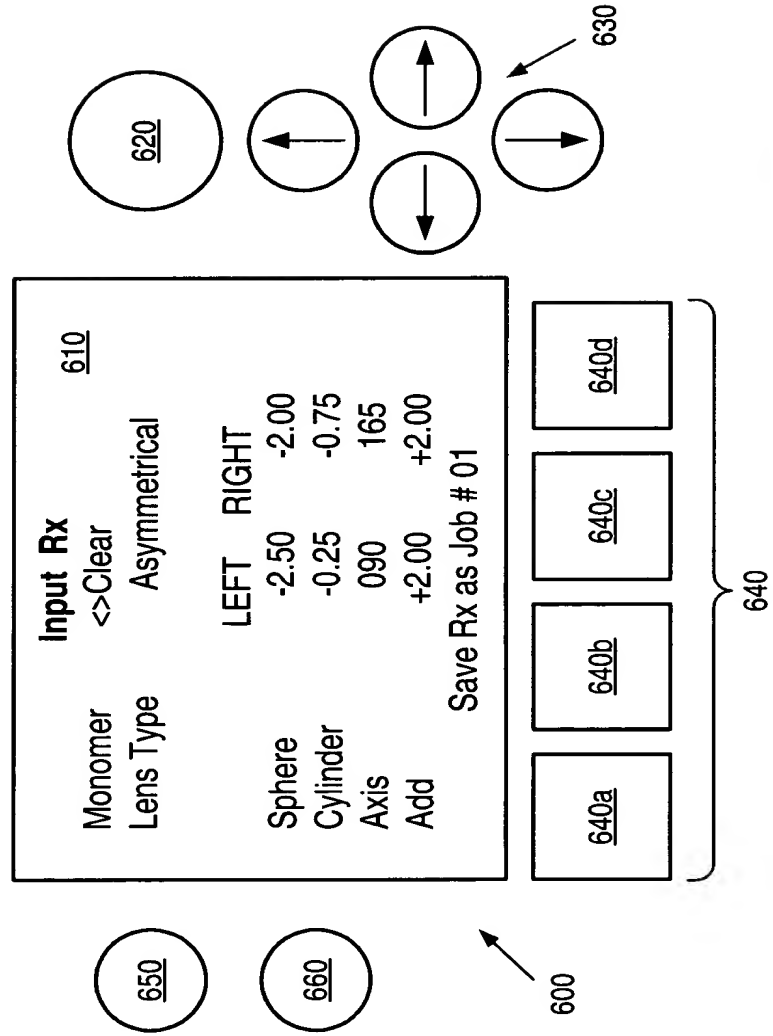


FIG. 18

50



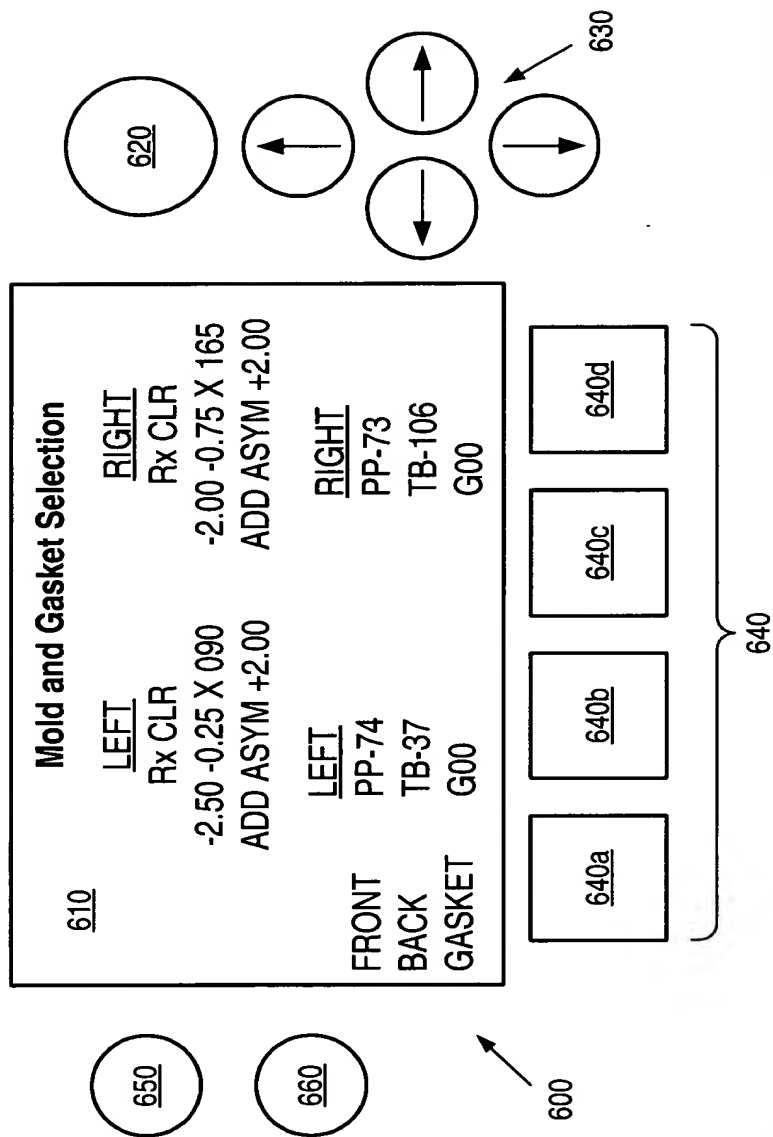


FIG. 19

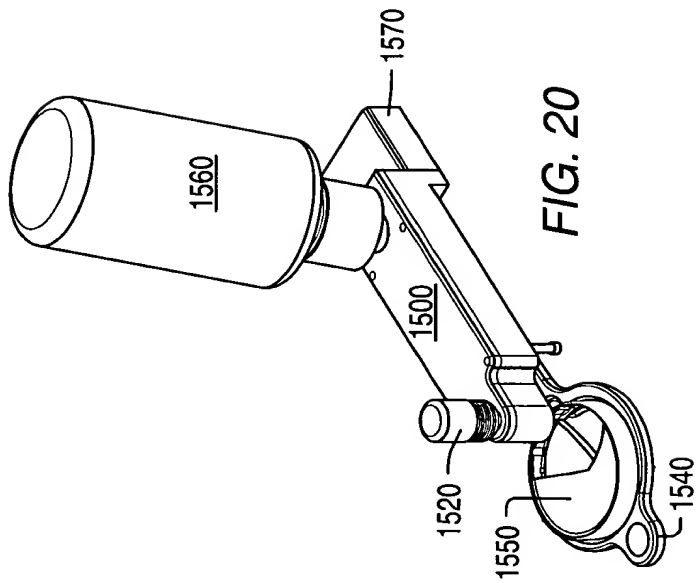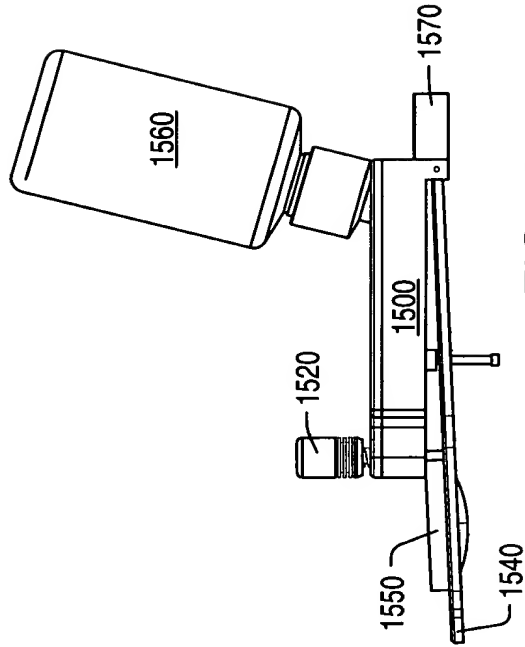

15/42

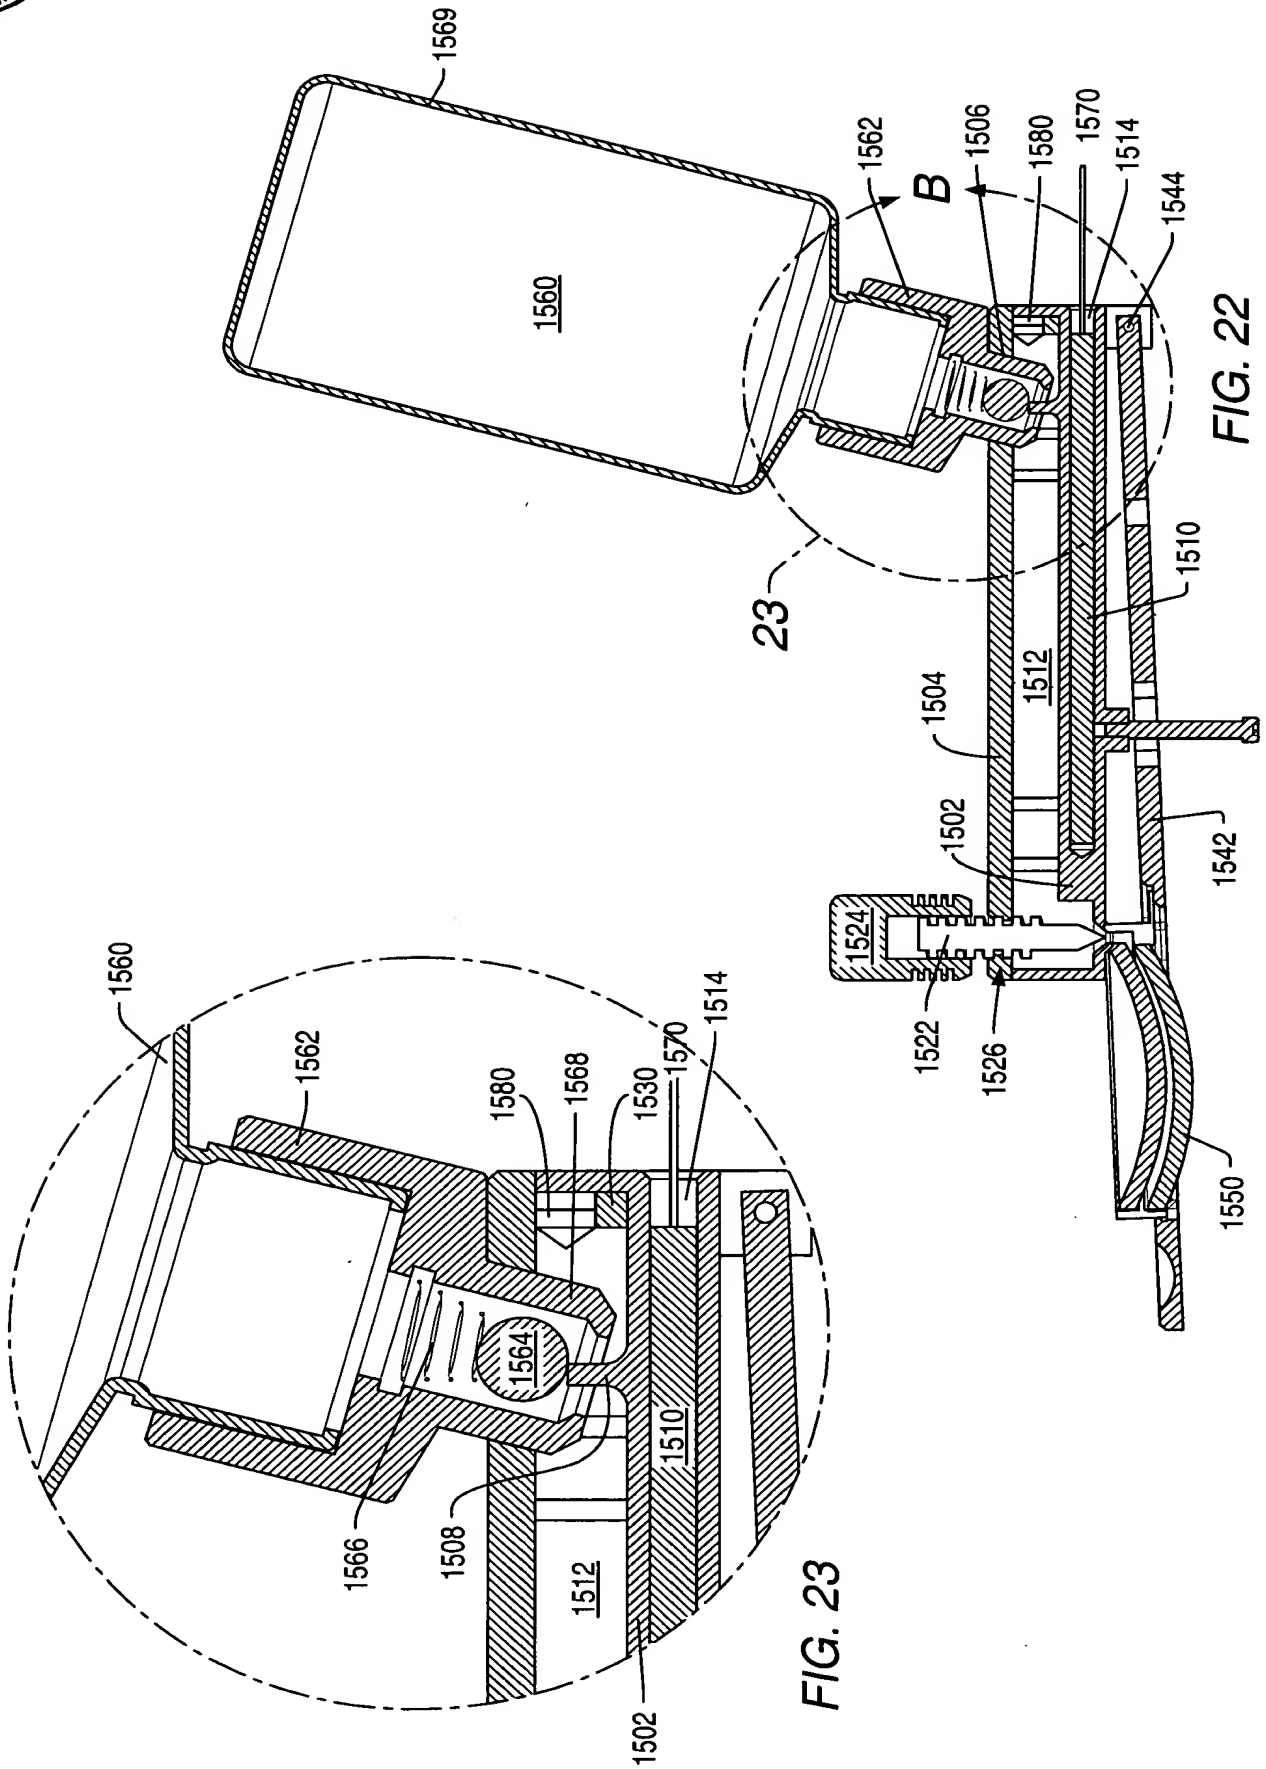


FIG. 23

FIG. 22



16/42

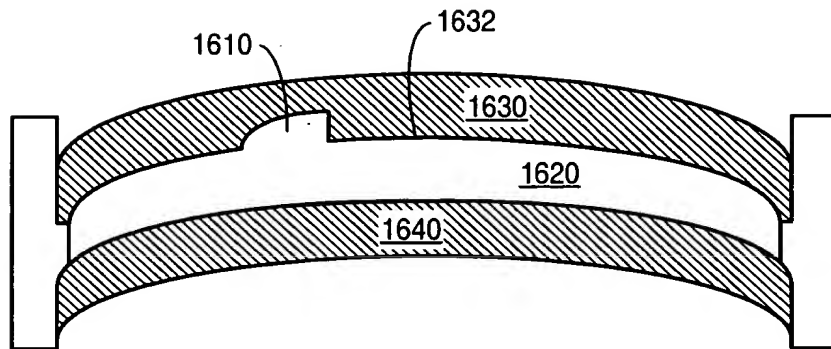


FIG. 24

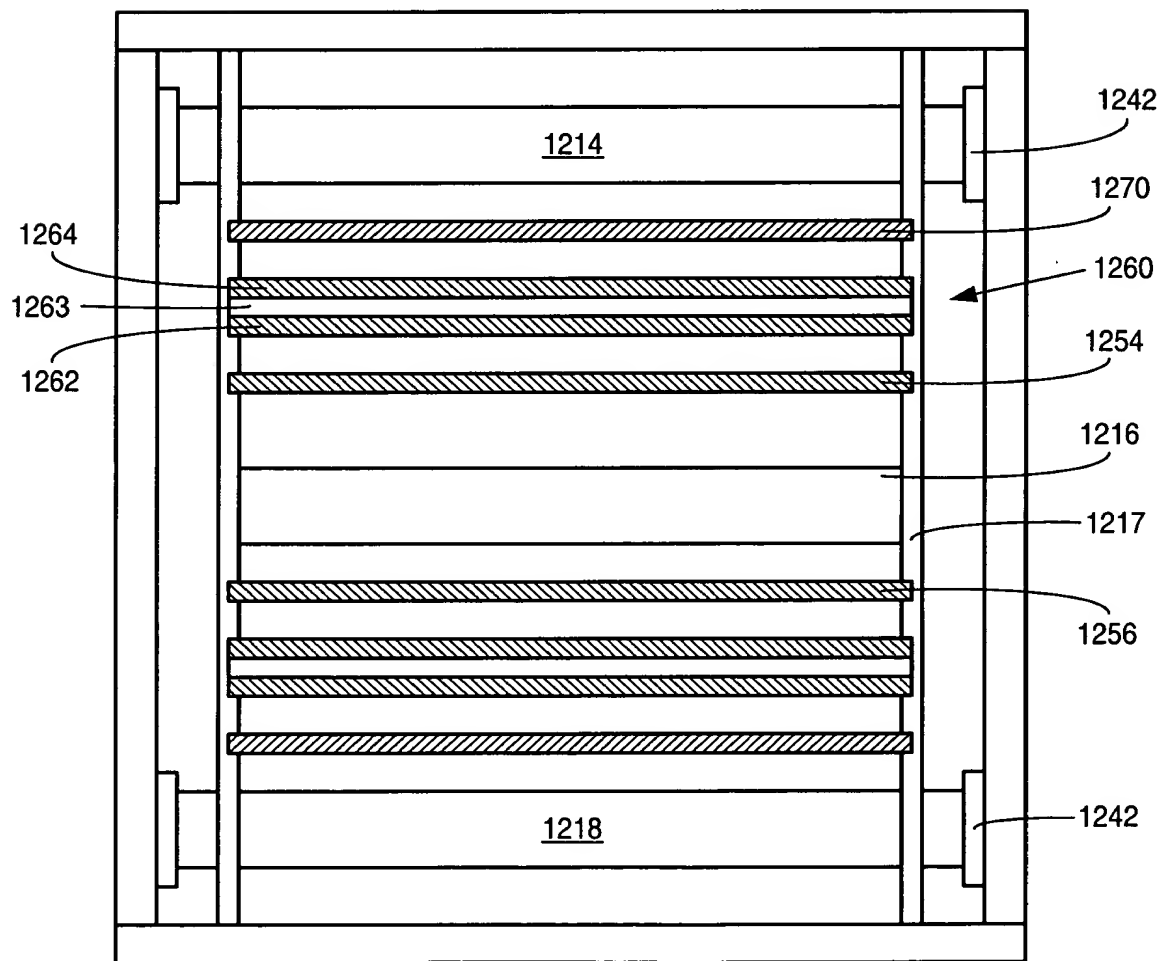


FIG. 25

1230



17/42

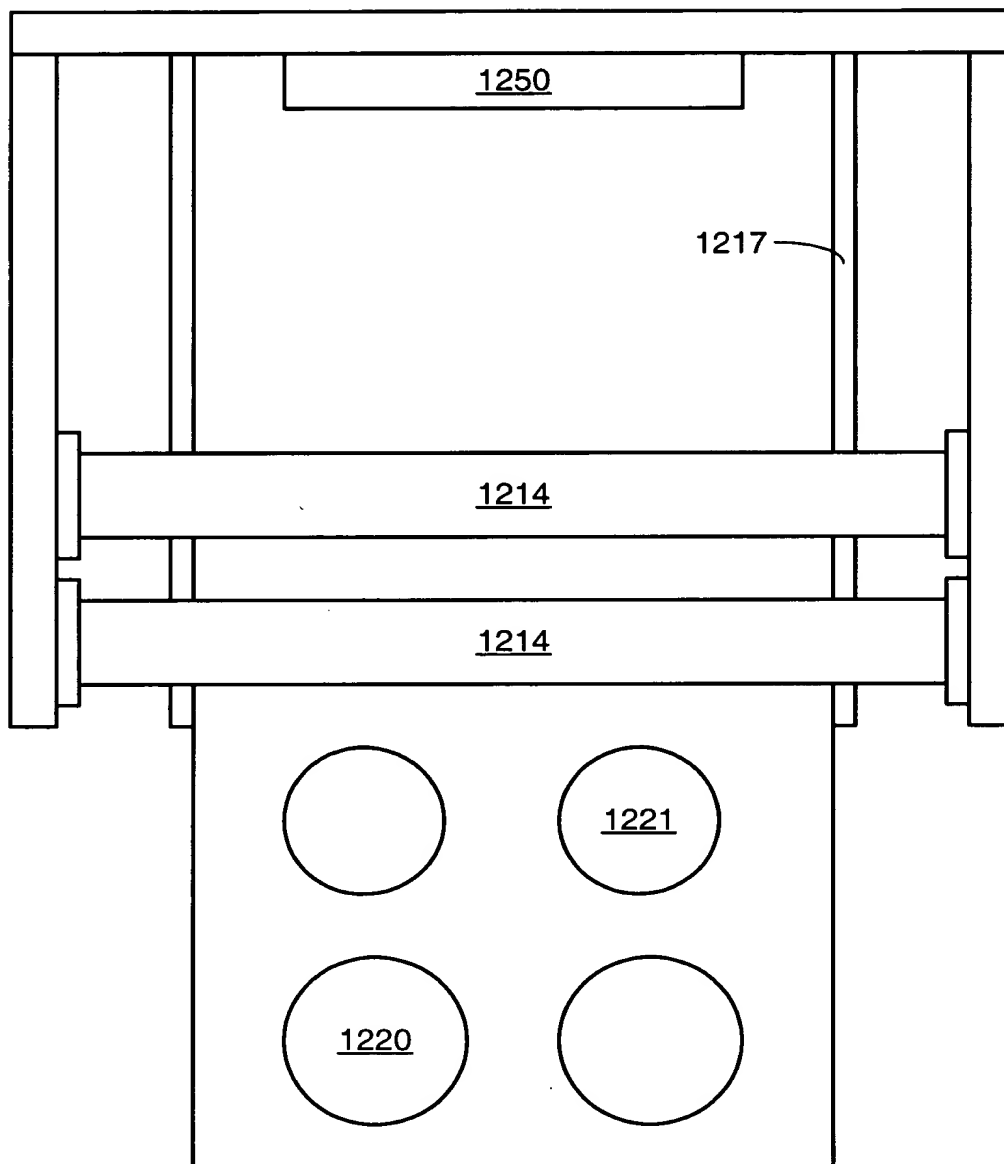


FIG. 26



18/42

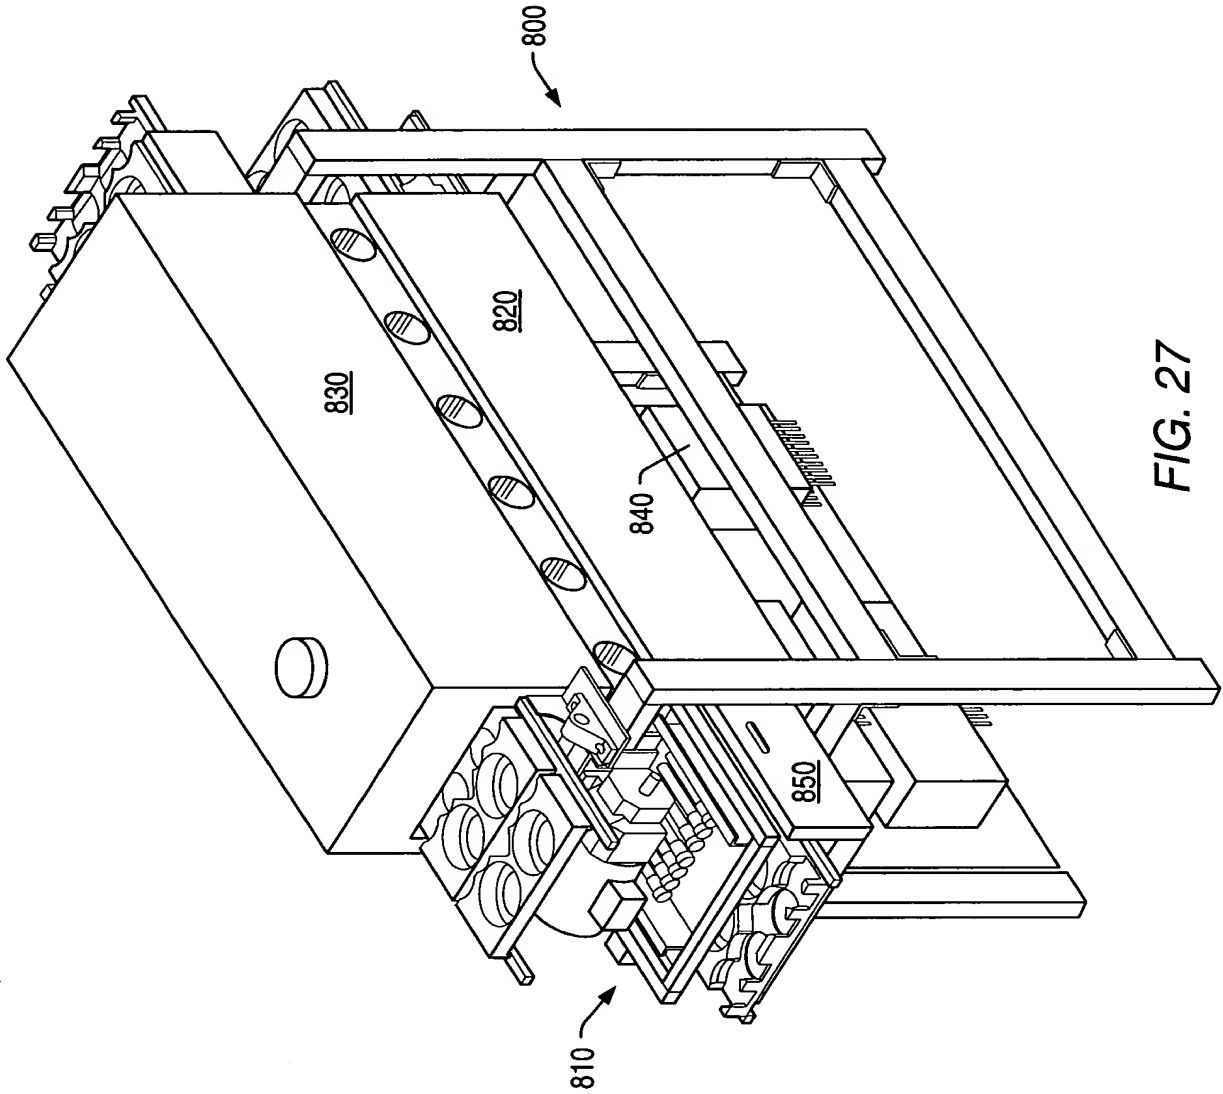


FIG. 27



19/42

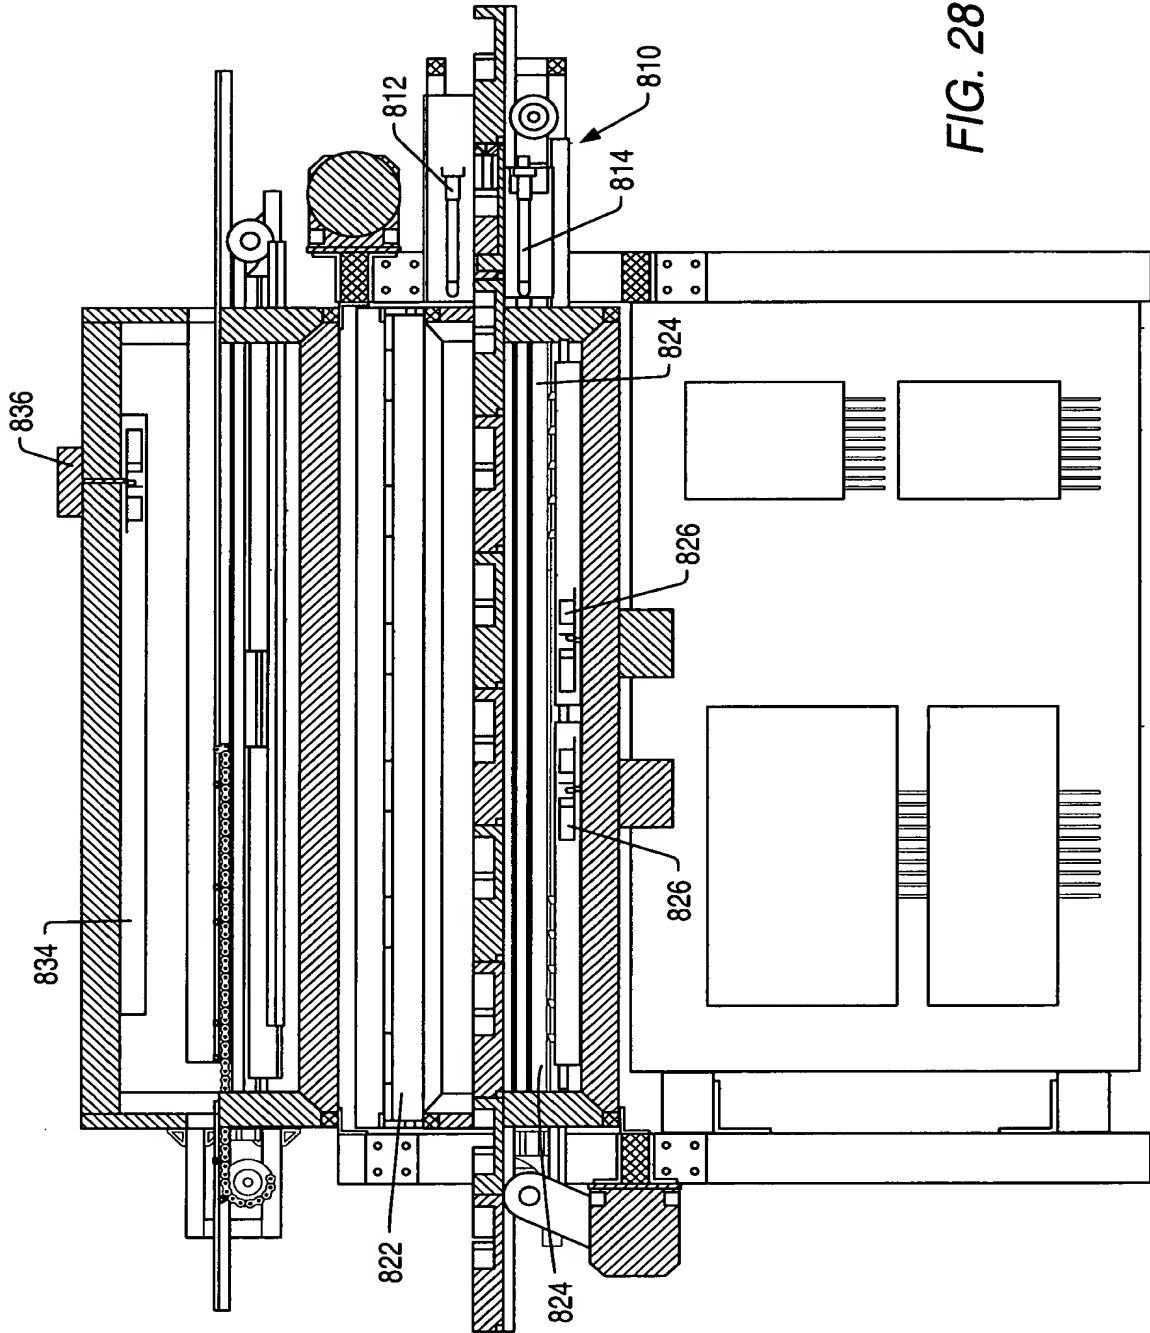


FIG. 28



20/42

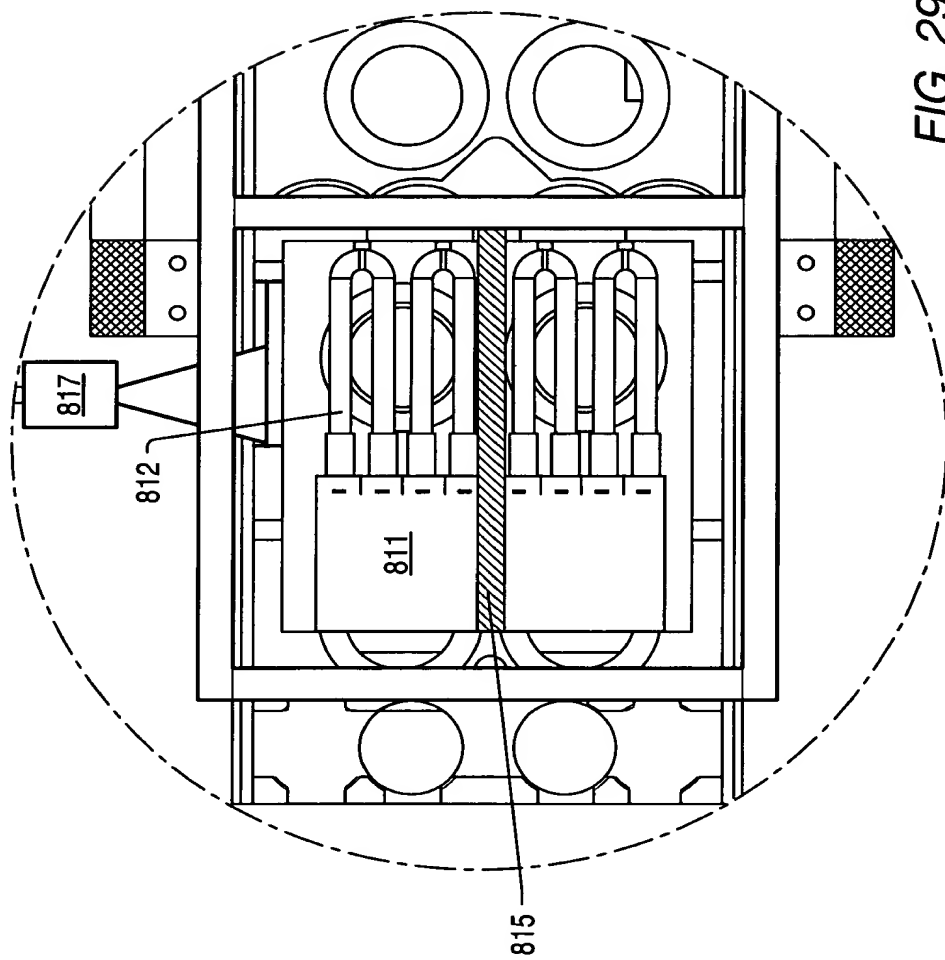


FIG. 29

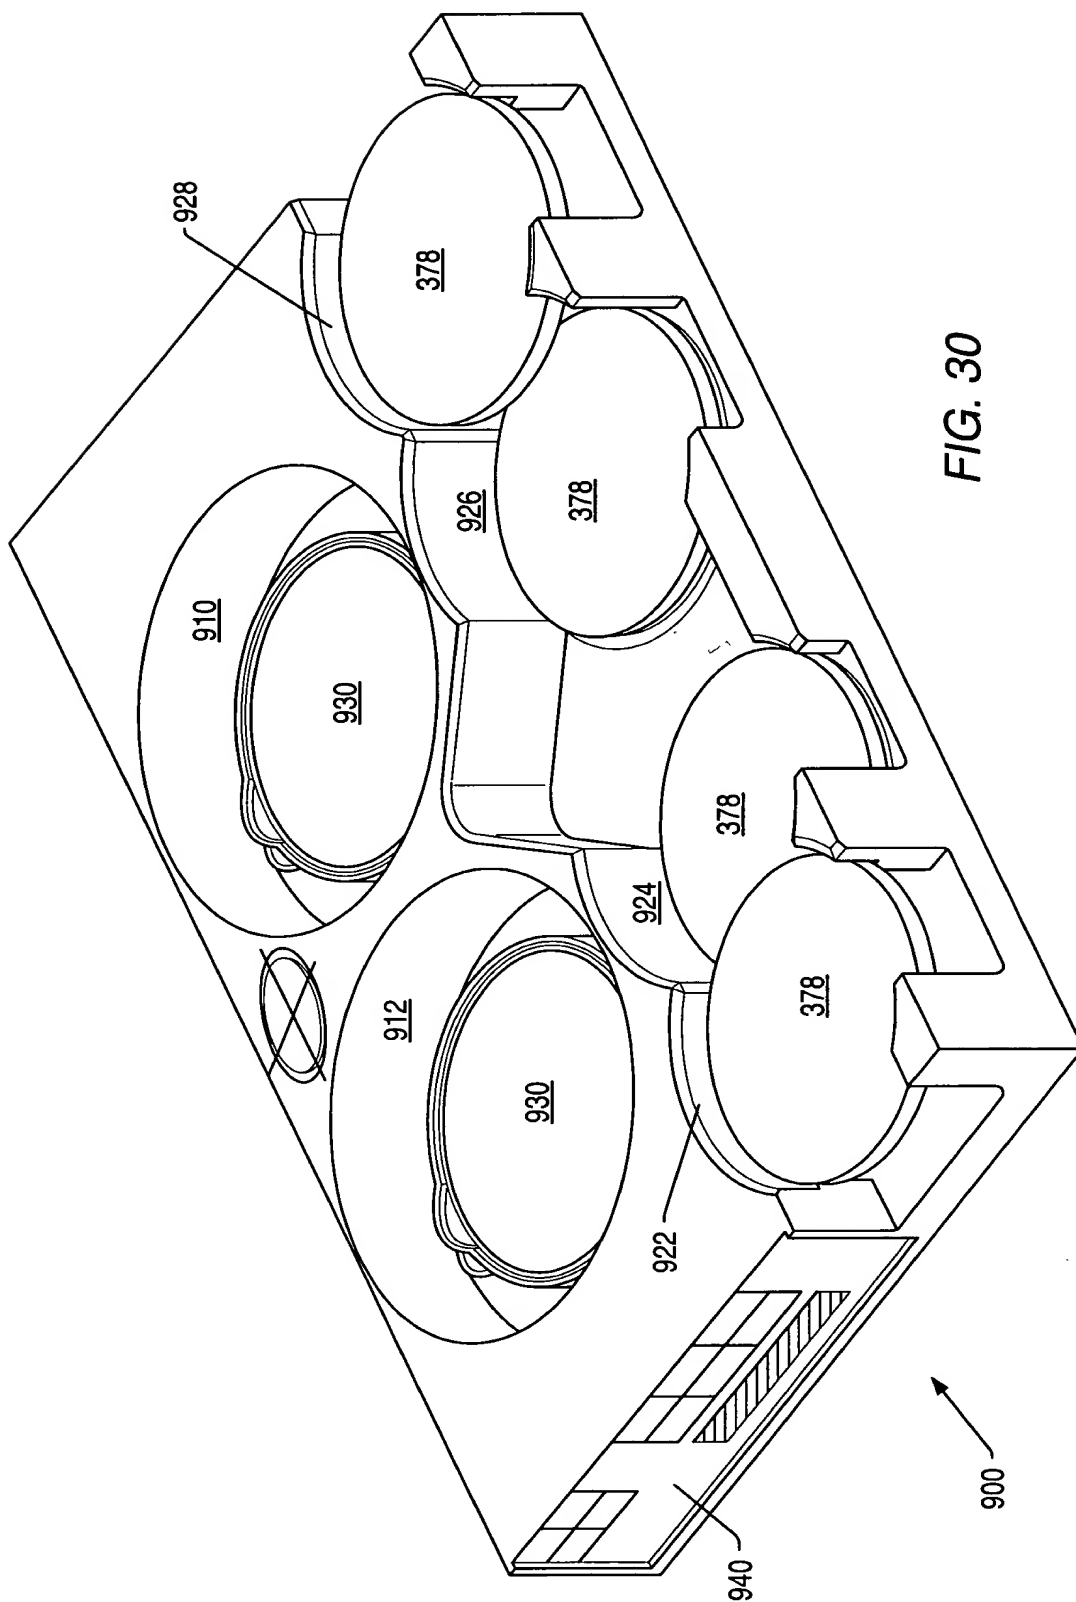


FIG. 30



22/42

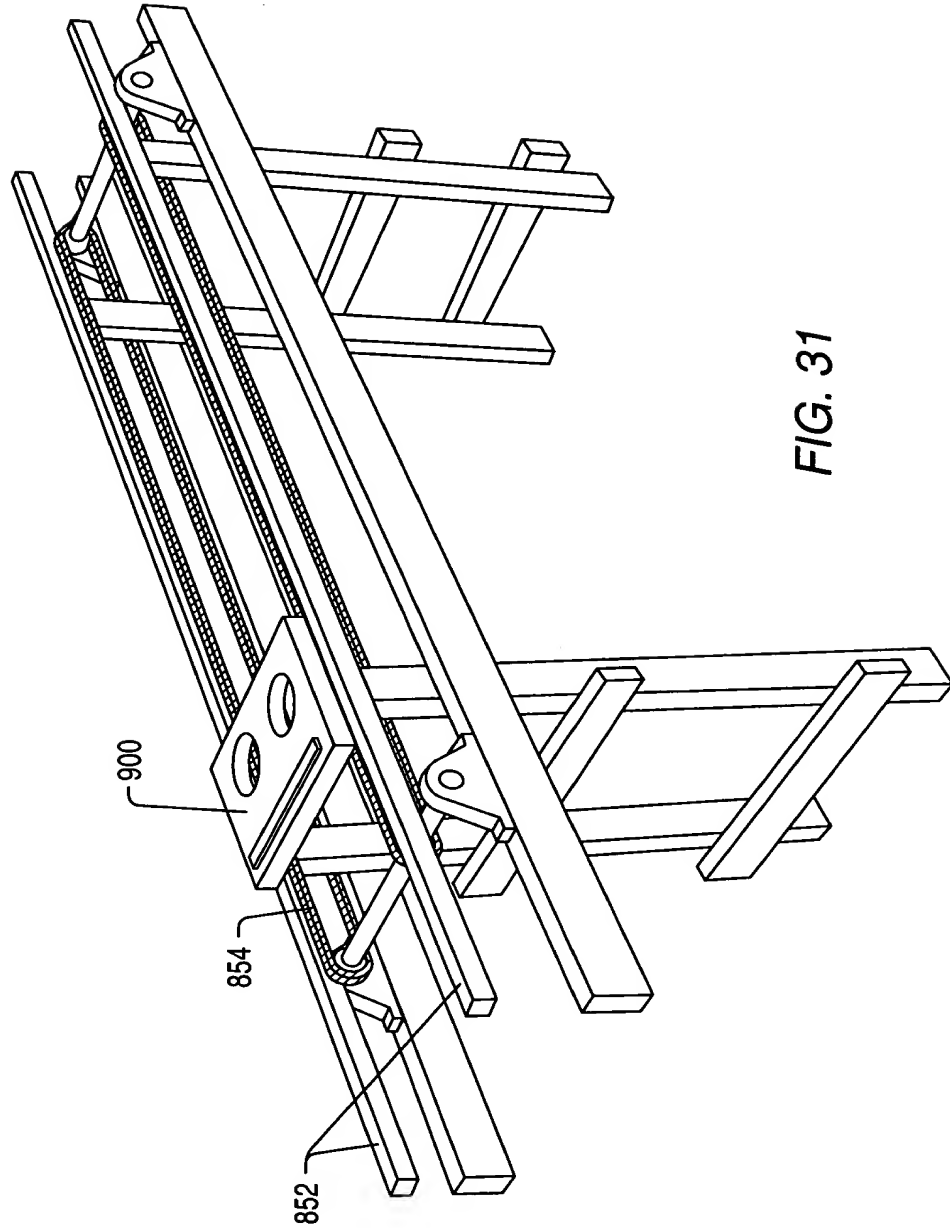


FIG. 31

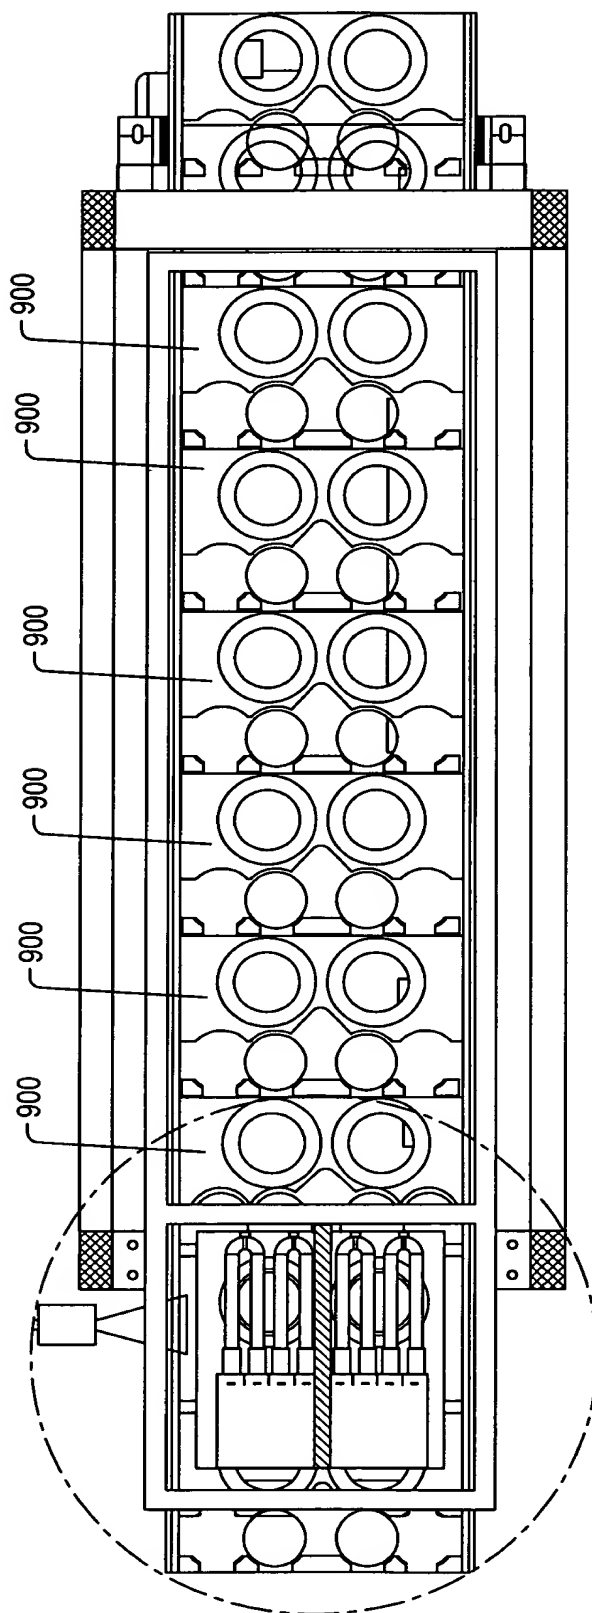


FIG. 32

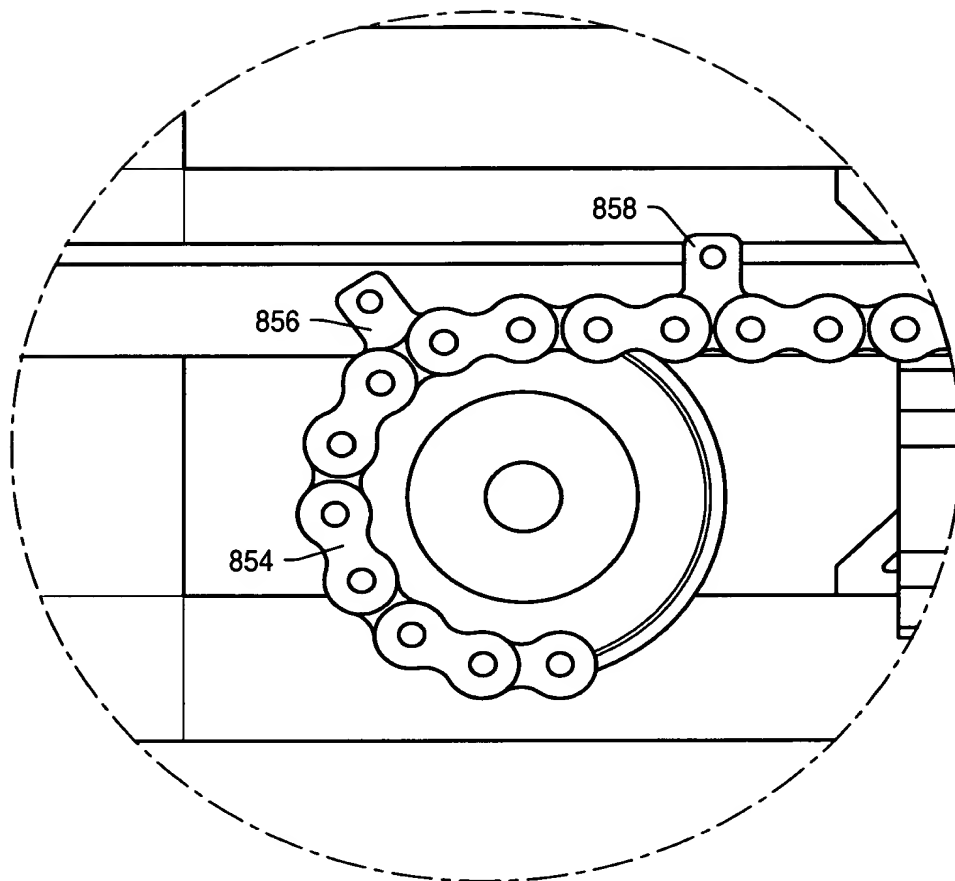


FIG. 33

25/42

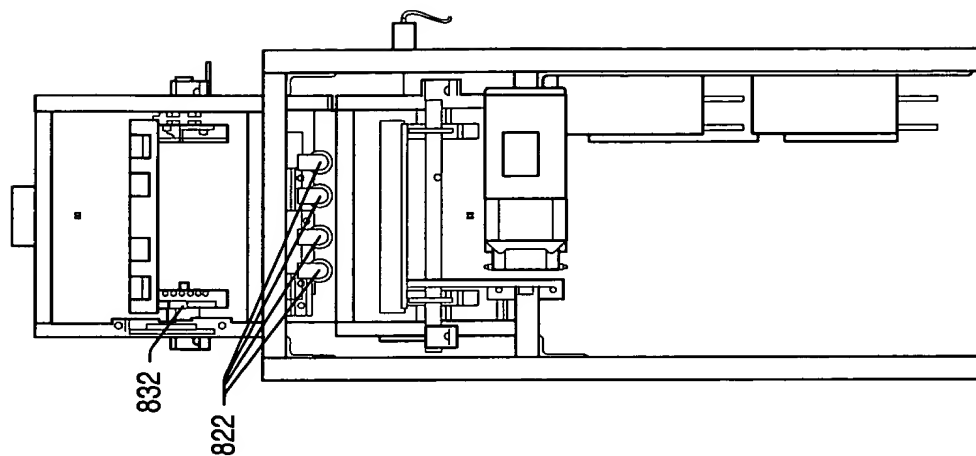


FIG. 35

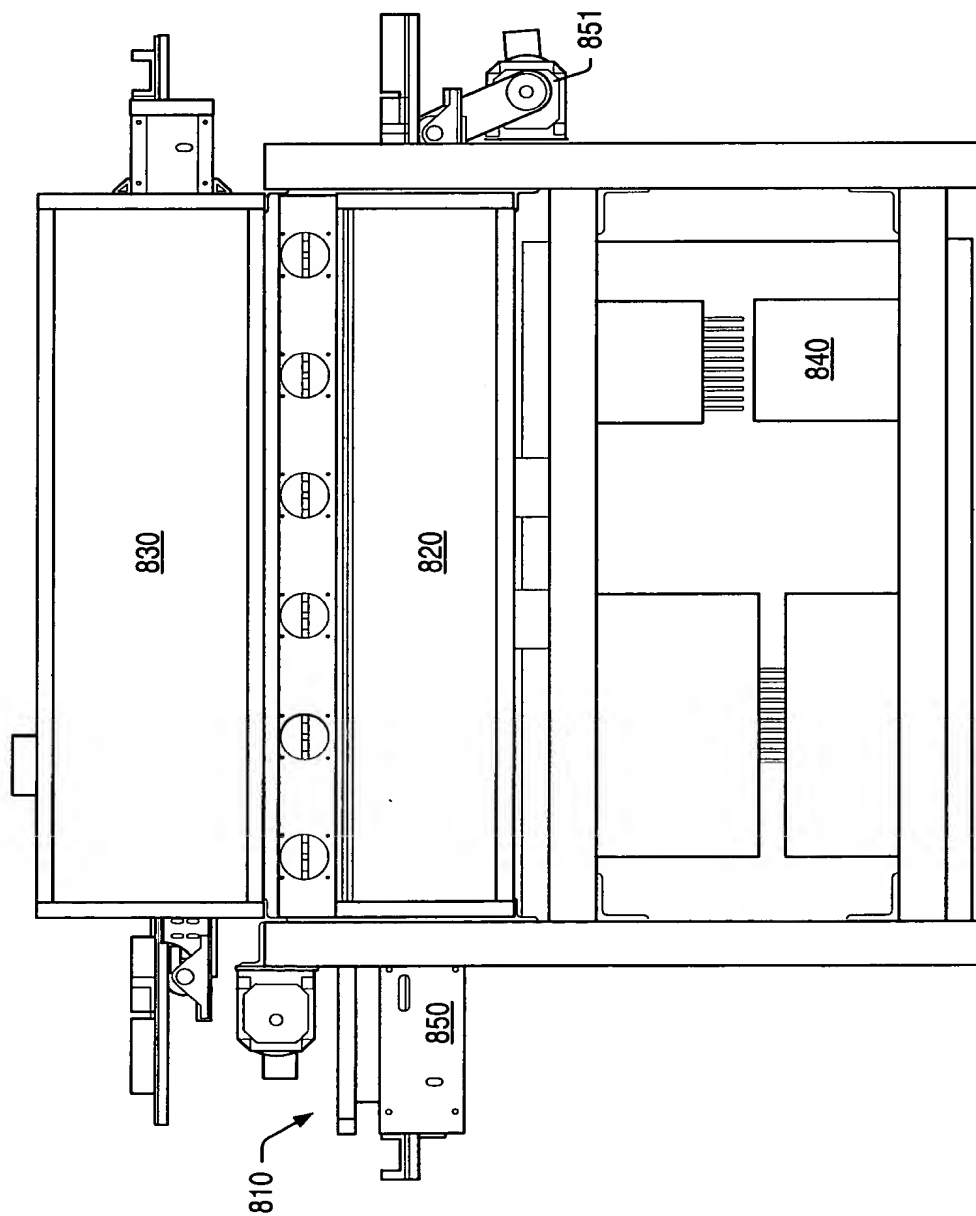


FIG. 34


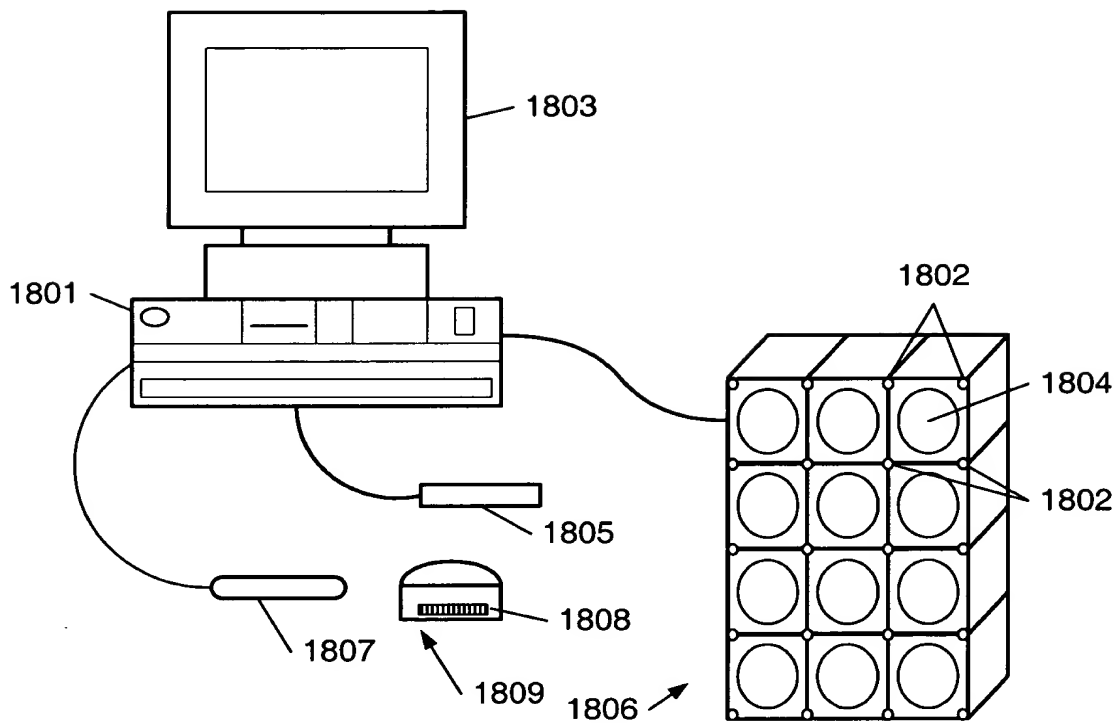



FIG. 36



27/42

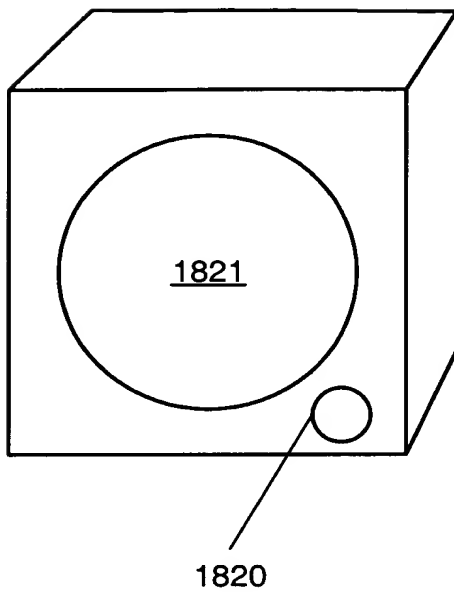

(a)

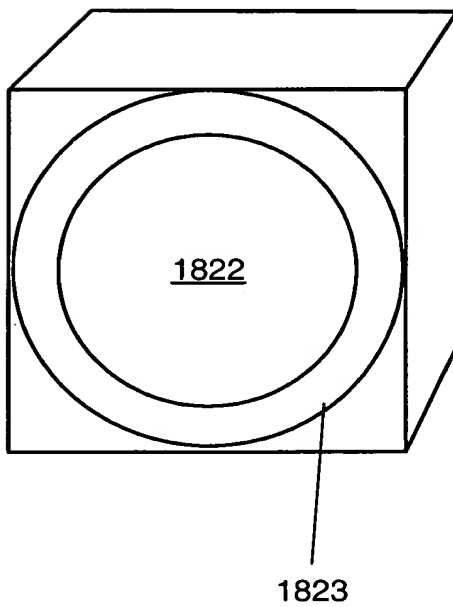

(b)

FIG. 37


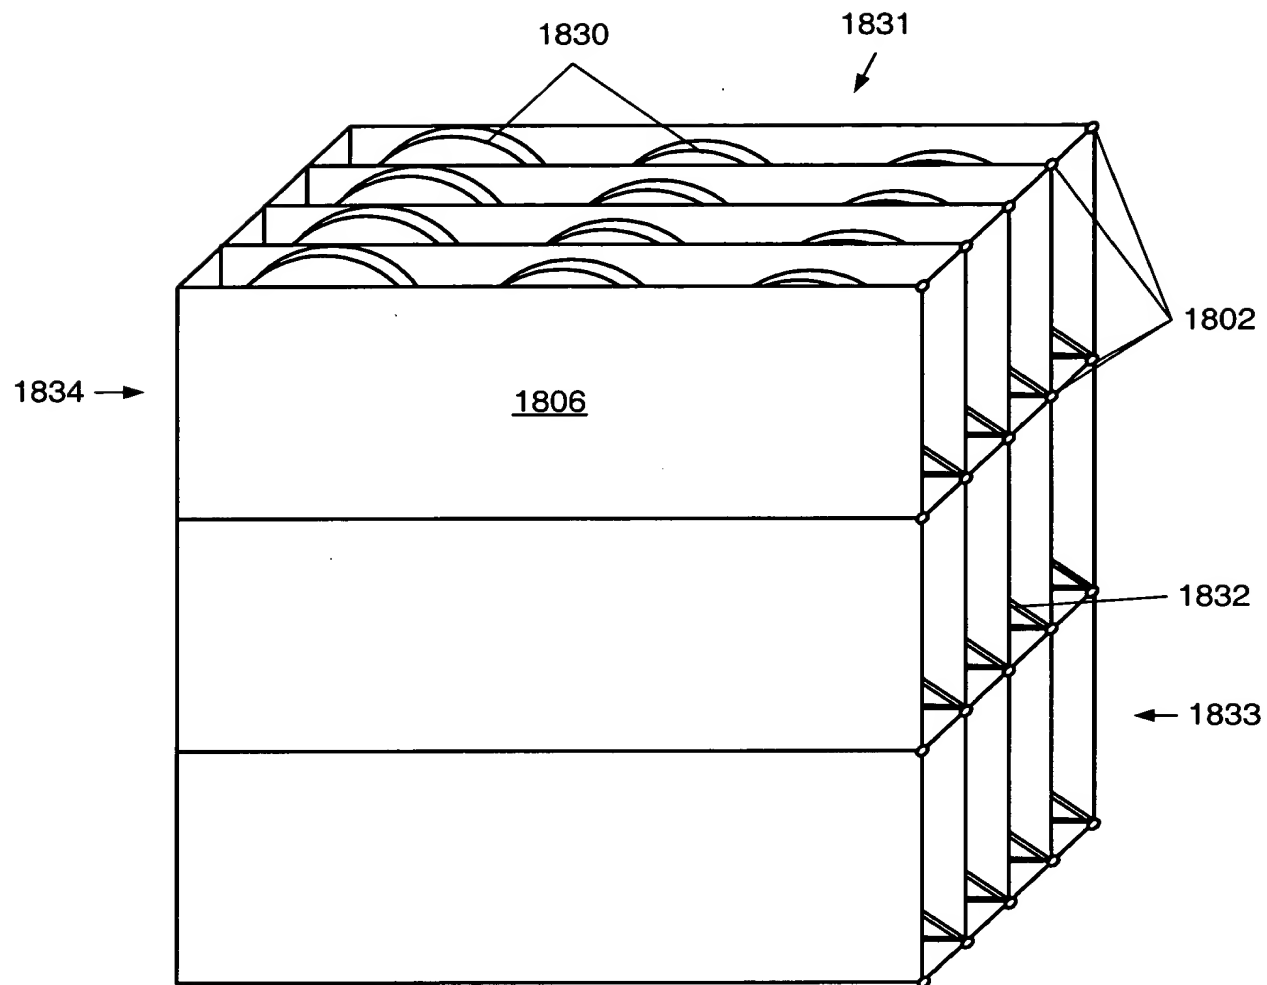


FIG. 38



29/42

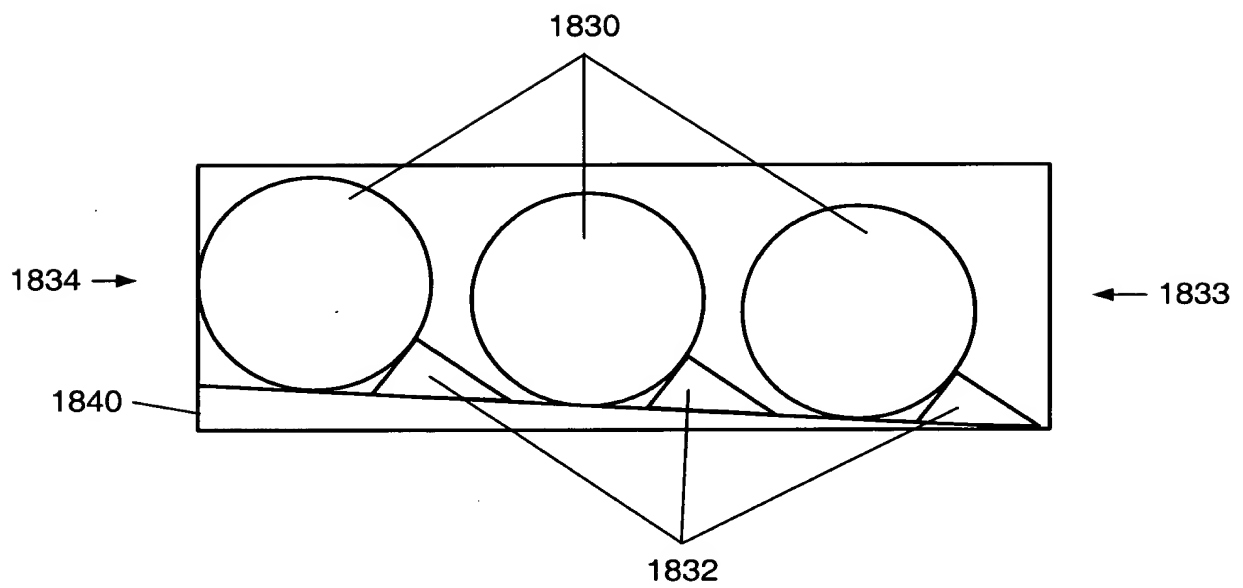


FIG. 39

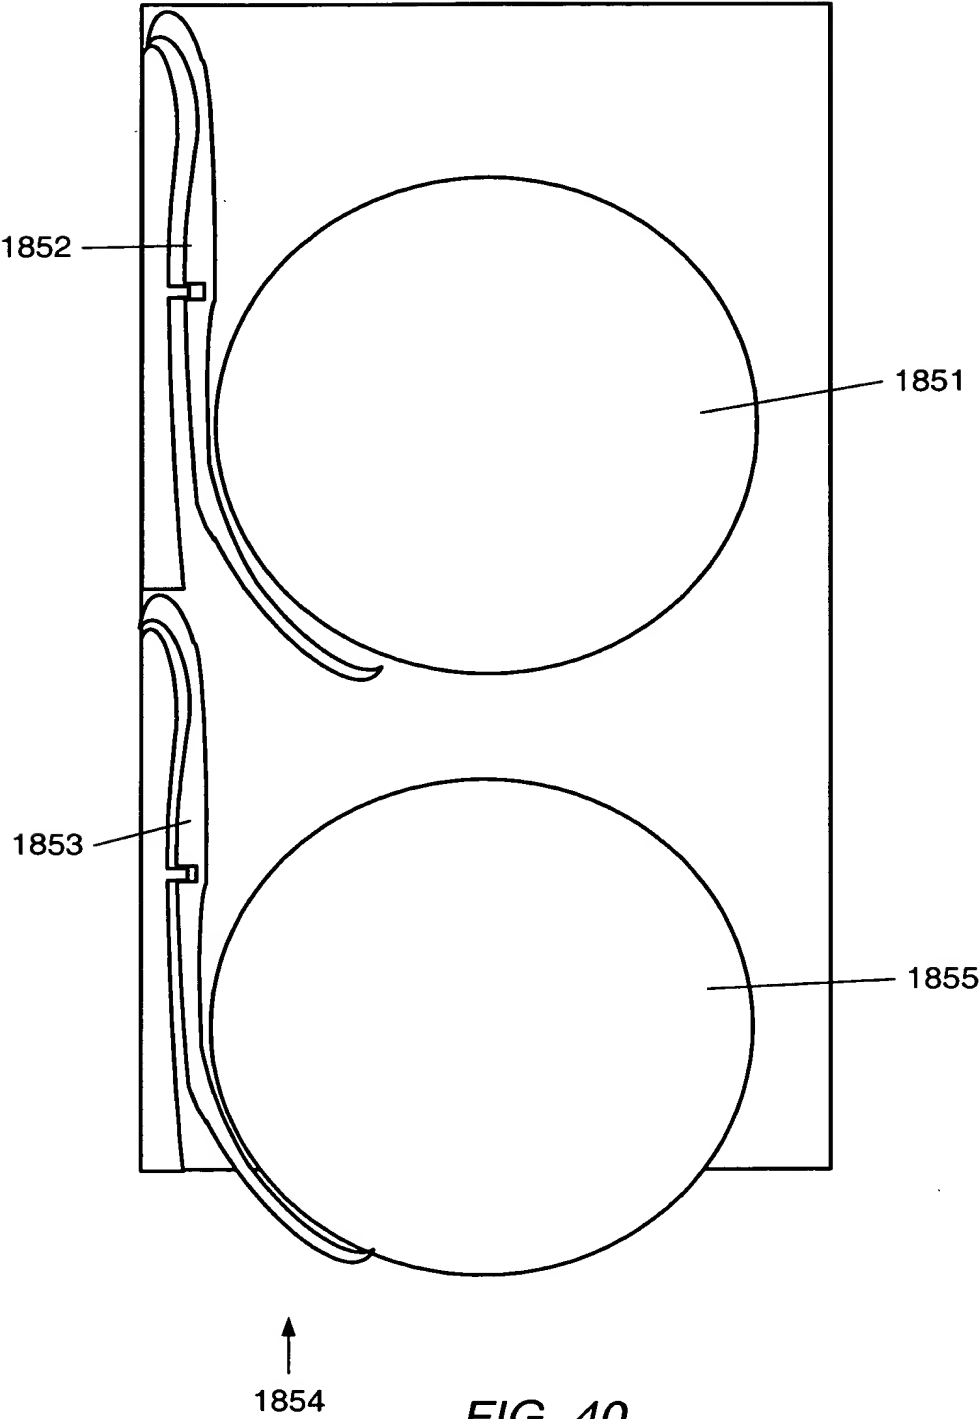


FIG. 40

31/42

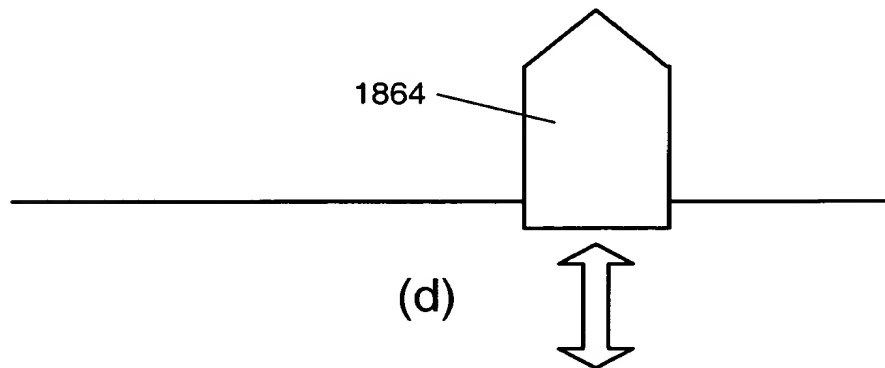
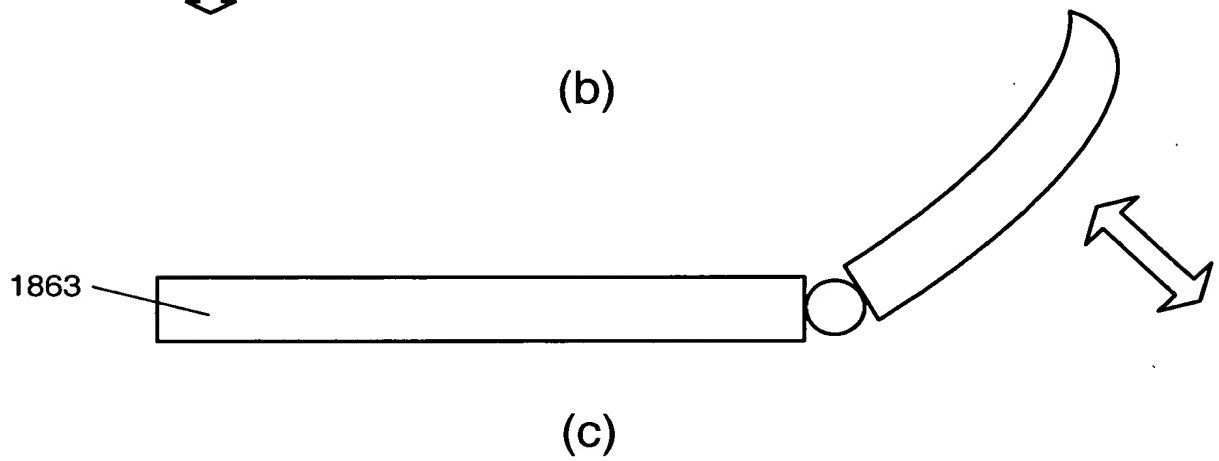
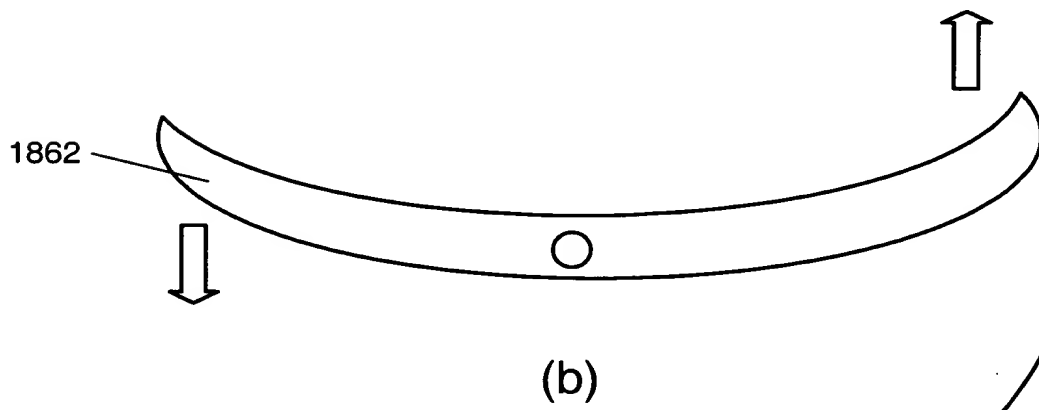
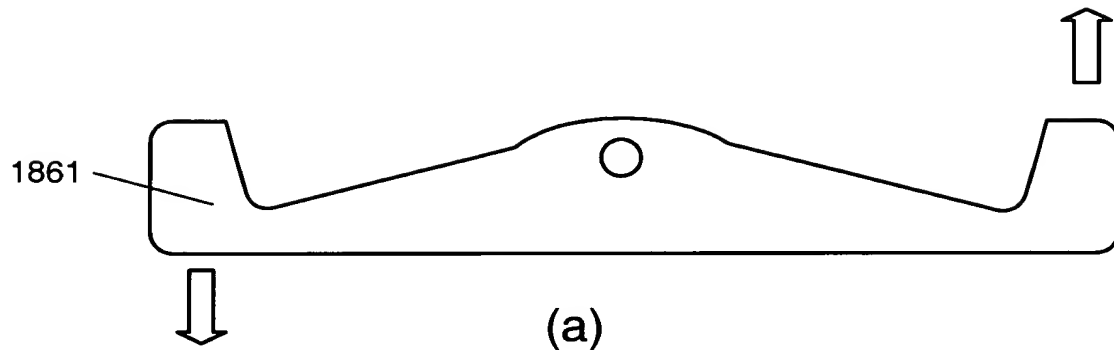


FIG. 41

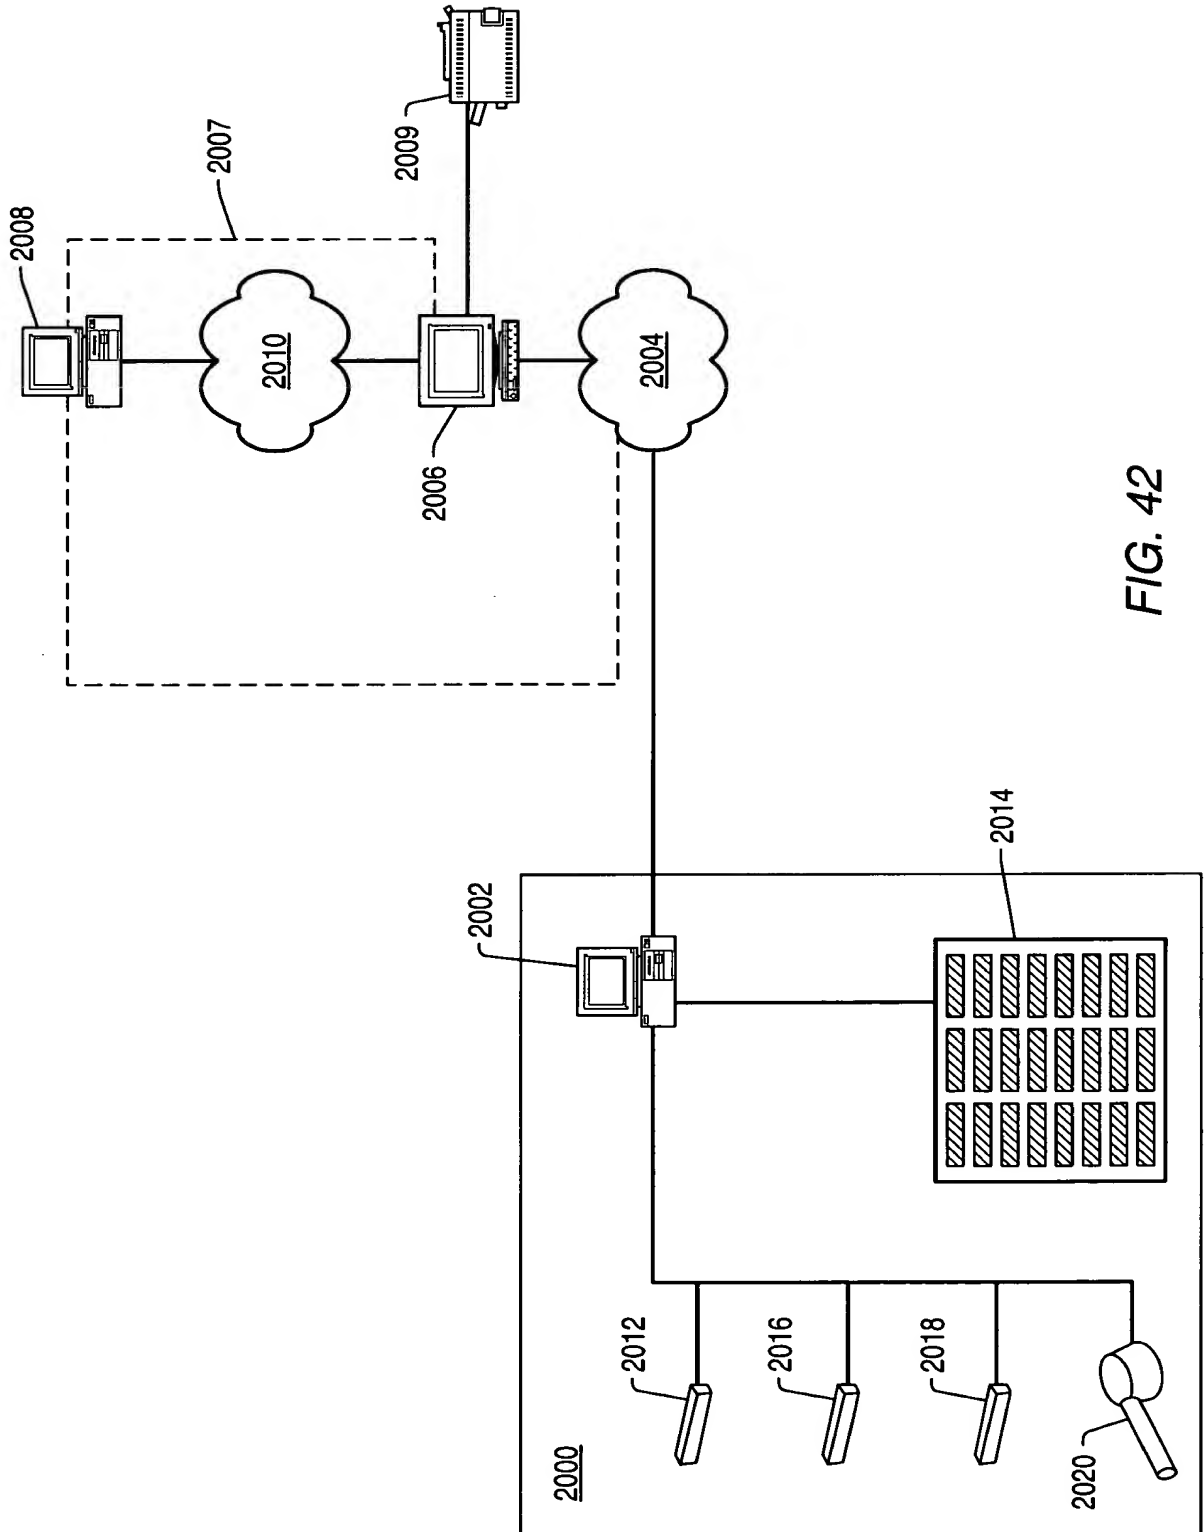


FIG. 42

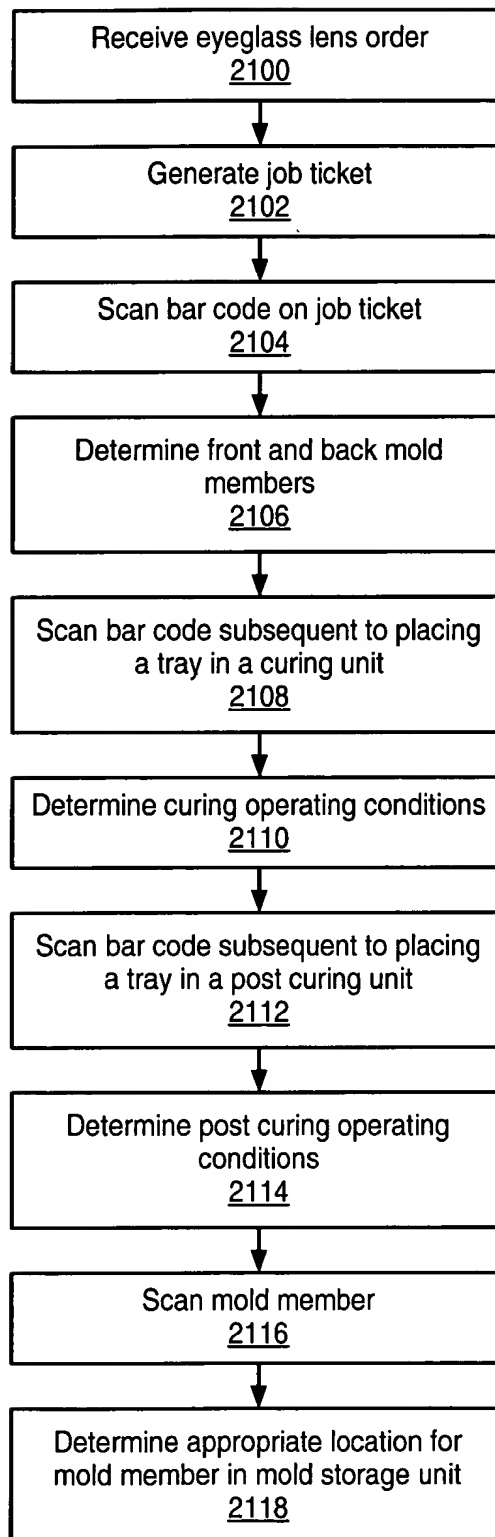
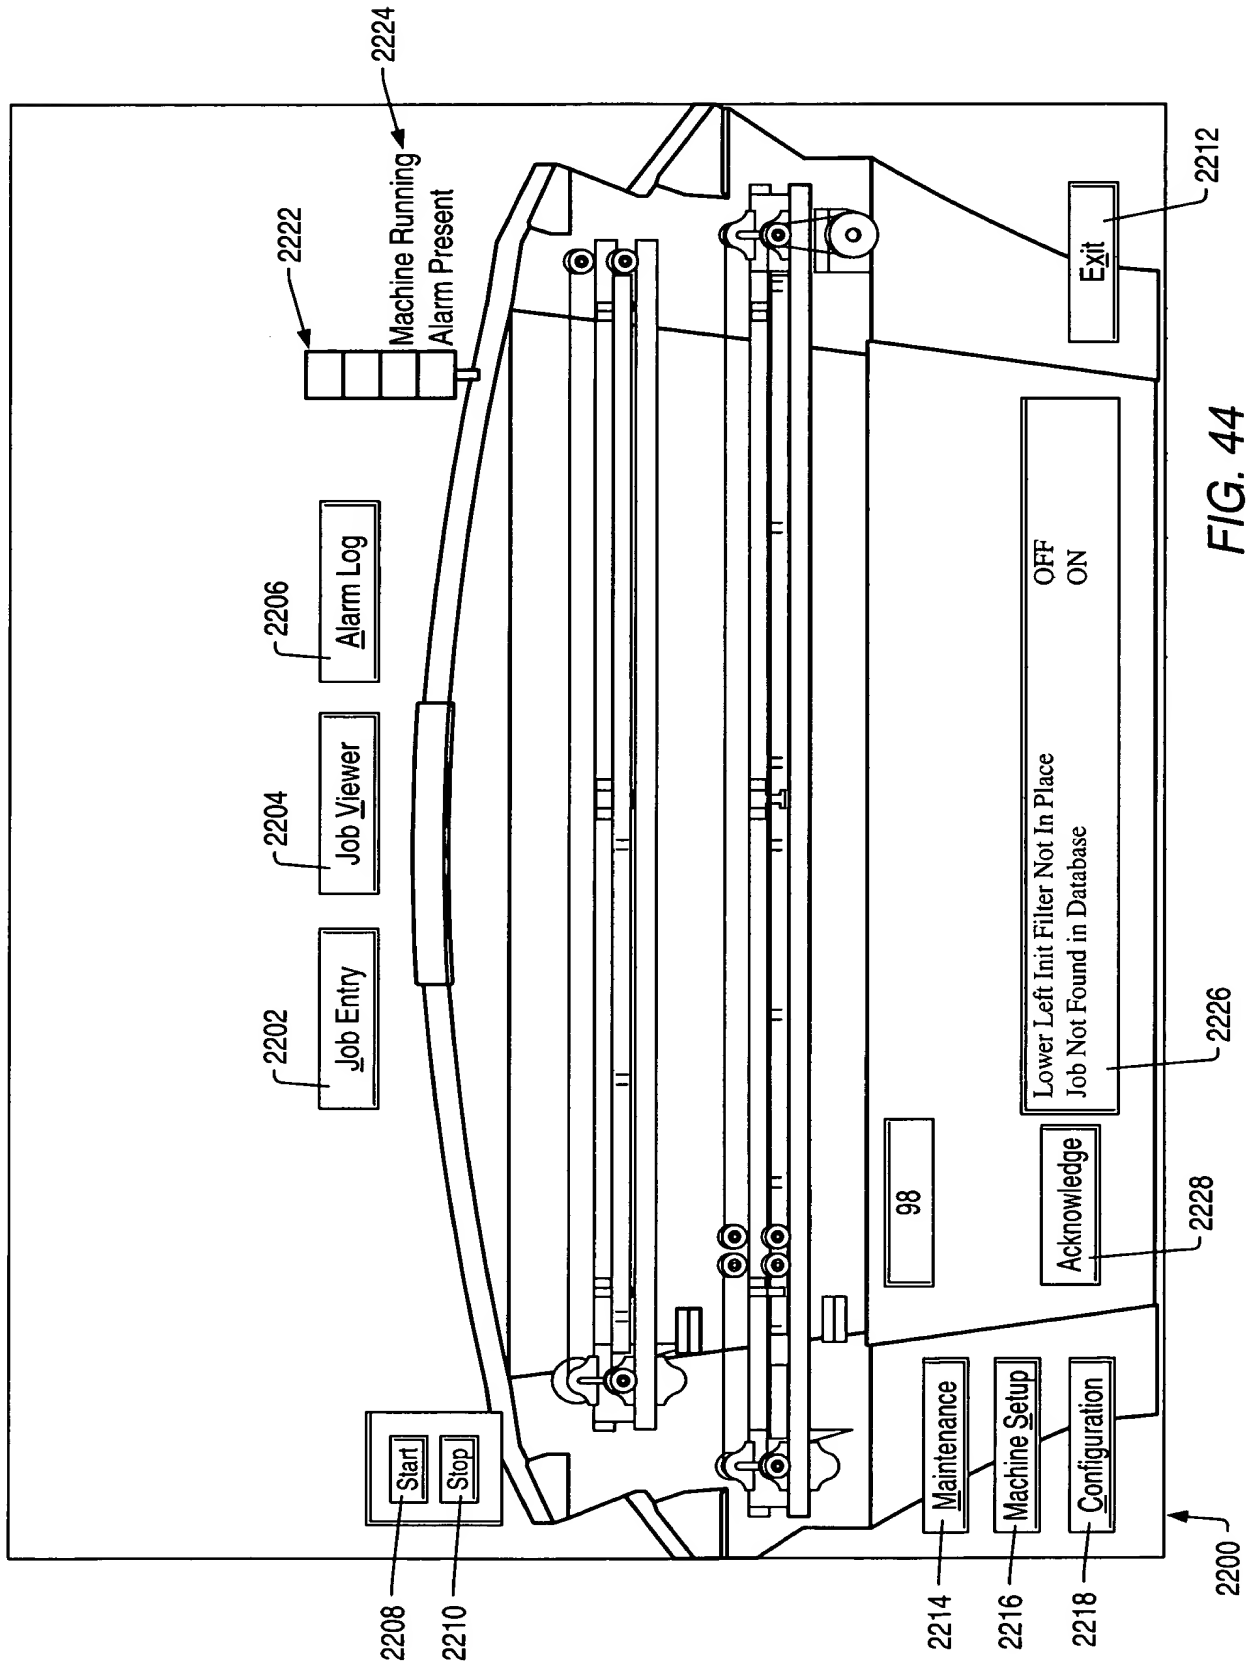


FIG. 43




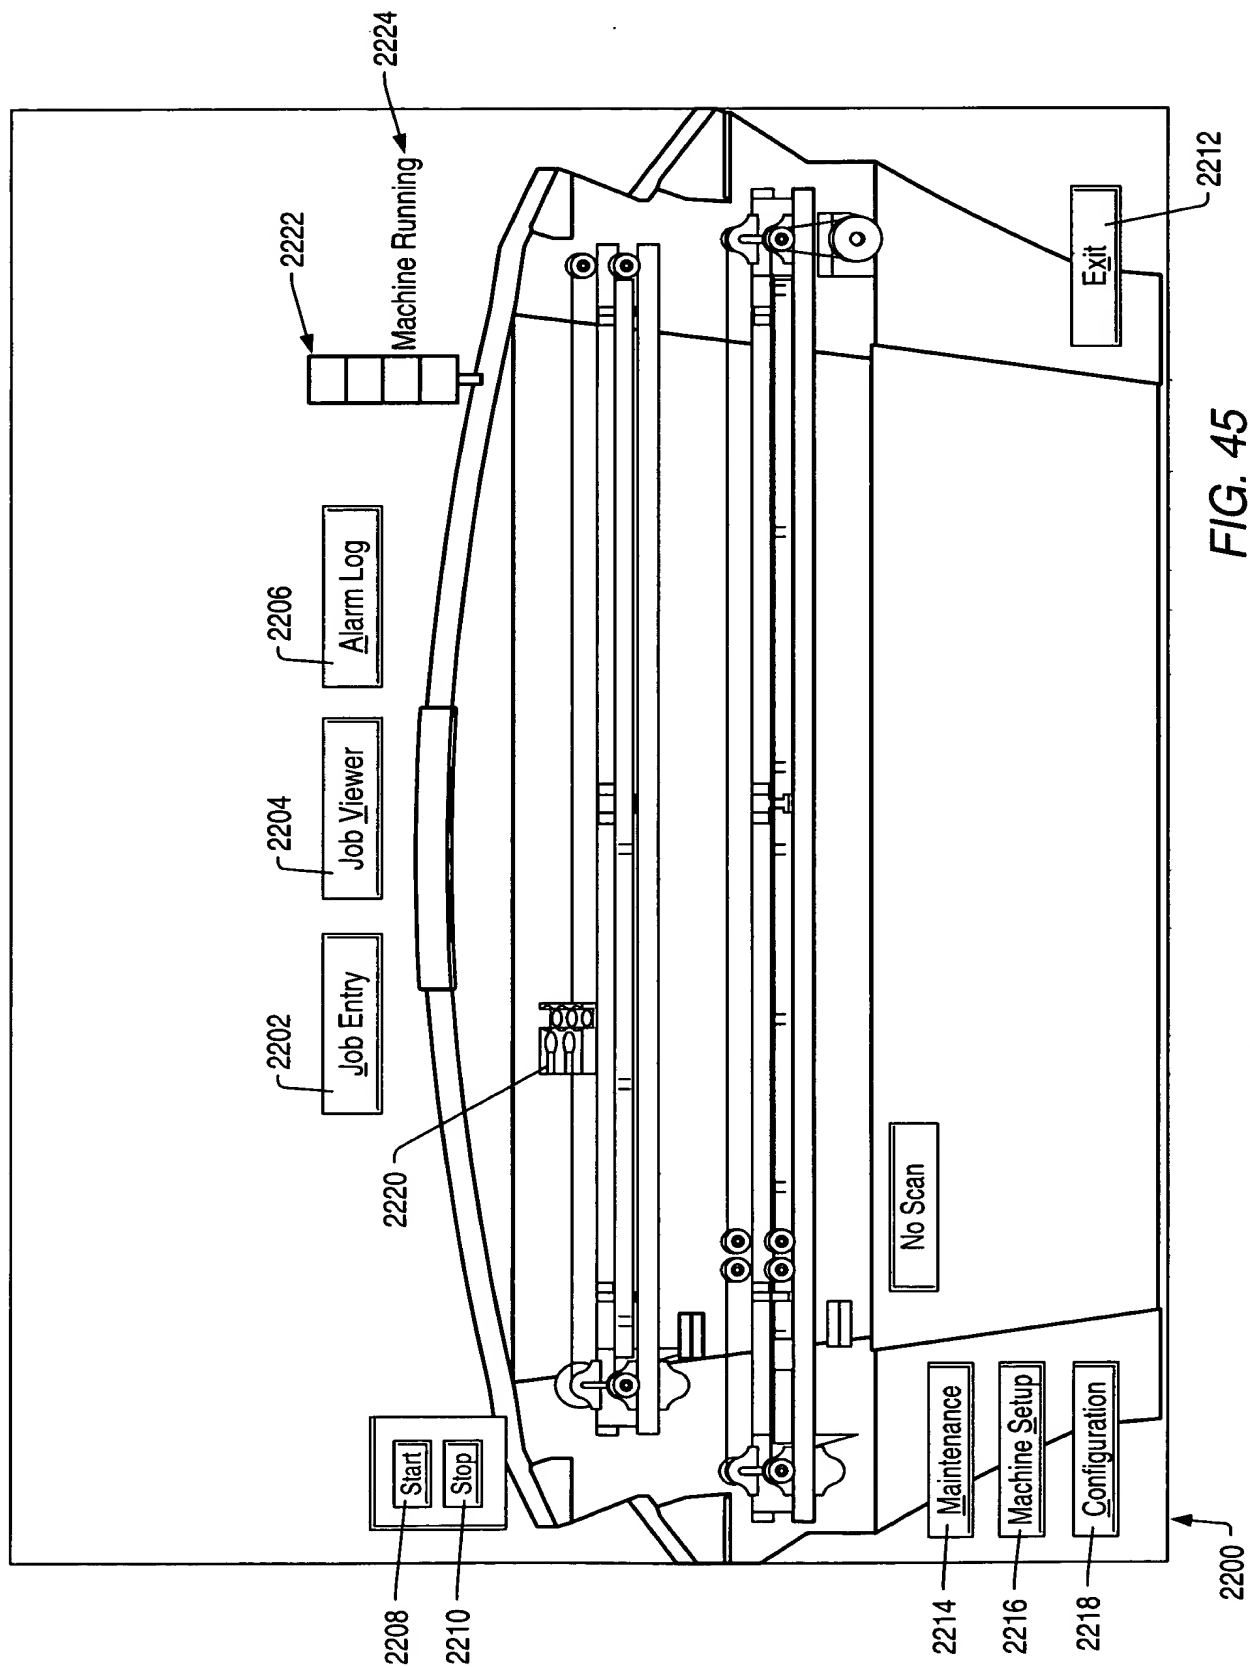


FIG. 45

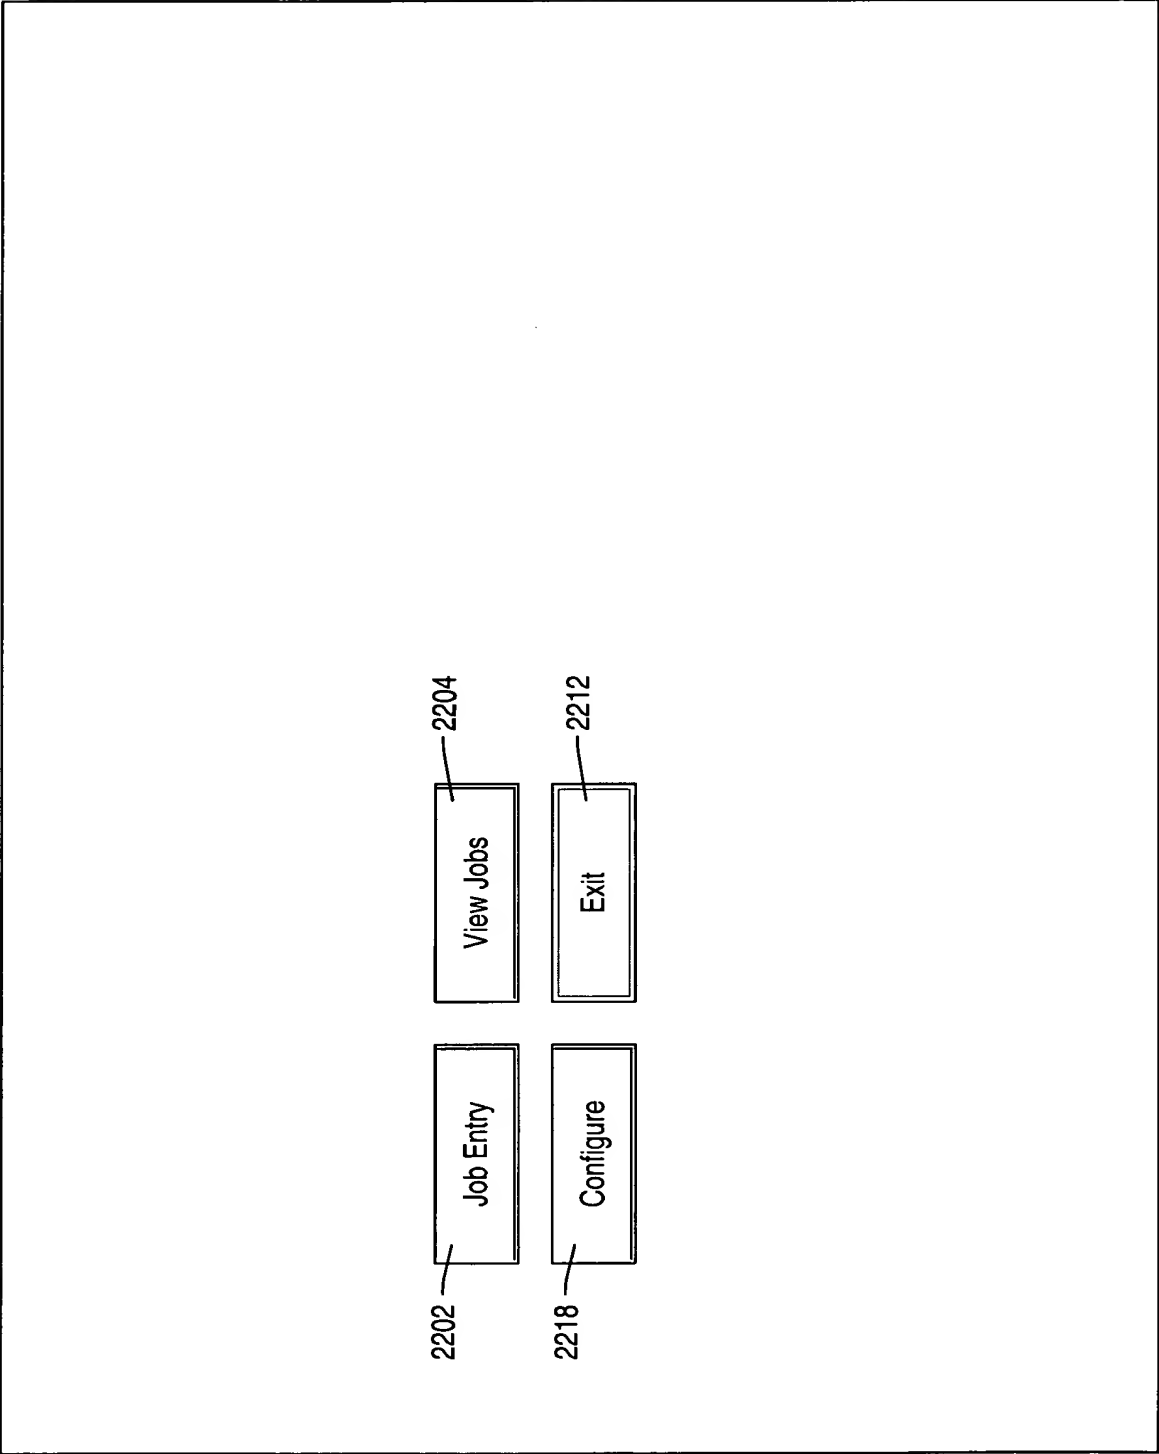

2228

FIG. 46

Job Entry

Job #

Priority

☒ **Normal**
☐ **Re-Work**

Patient Name

Tray #

Bin Location

2232

Job Type

☒ **Right & Left Lens**
☐ **Right Lens Only**
☐ **Left Lens Only**

Lens Type

☒ **Aspheric - Single Vision**
☐ **Flat Top**
☐ **Paradigm Progressive**

Monomer/Tint

☐ **Clear**
☒ **Clear w/Tint**
☐ **Grey**

Right Eye

Sphere

Cylinder

Left Eye

Sphere

Cylinder

2236

2238

2240

2230

FIG. 47



Job Viewer

LMS Job # 2244

Patient

LMS Tray #

Entry Date

Bin Location

Lens Type

Monomer

Rx

	Left	Right
Power	<input type="text" value="-6.00"/>	<input type="text"/>
Cylinder	<input type="text" value="-2.00"/>	<input type="text"/>
Axis	<input type="text"/>	<input type="text"/>
Add	<input type="text"/>	<input type="text"/>

Molds

	Left	Right
Front	<input type="text" value="No"/>	<input type="text"/>
Back	<input type="text" value="Rx"/>	<input type="text"/>
Gasket	<input type="text" value="Mold"/>	<input type="text"/>
Filter	<input type="text"/>	<input type="text"/>
Recipe	<input type="text"/>	<input type="text"/>

Re-Print 2248

Close 2280

2242

FIG. 48

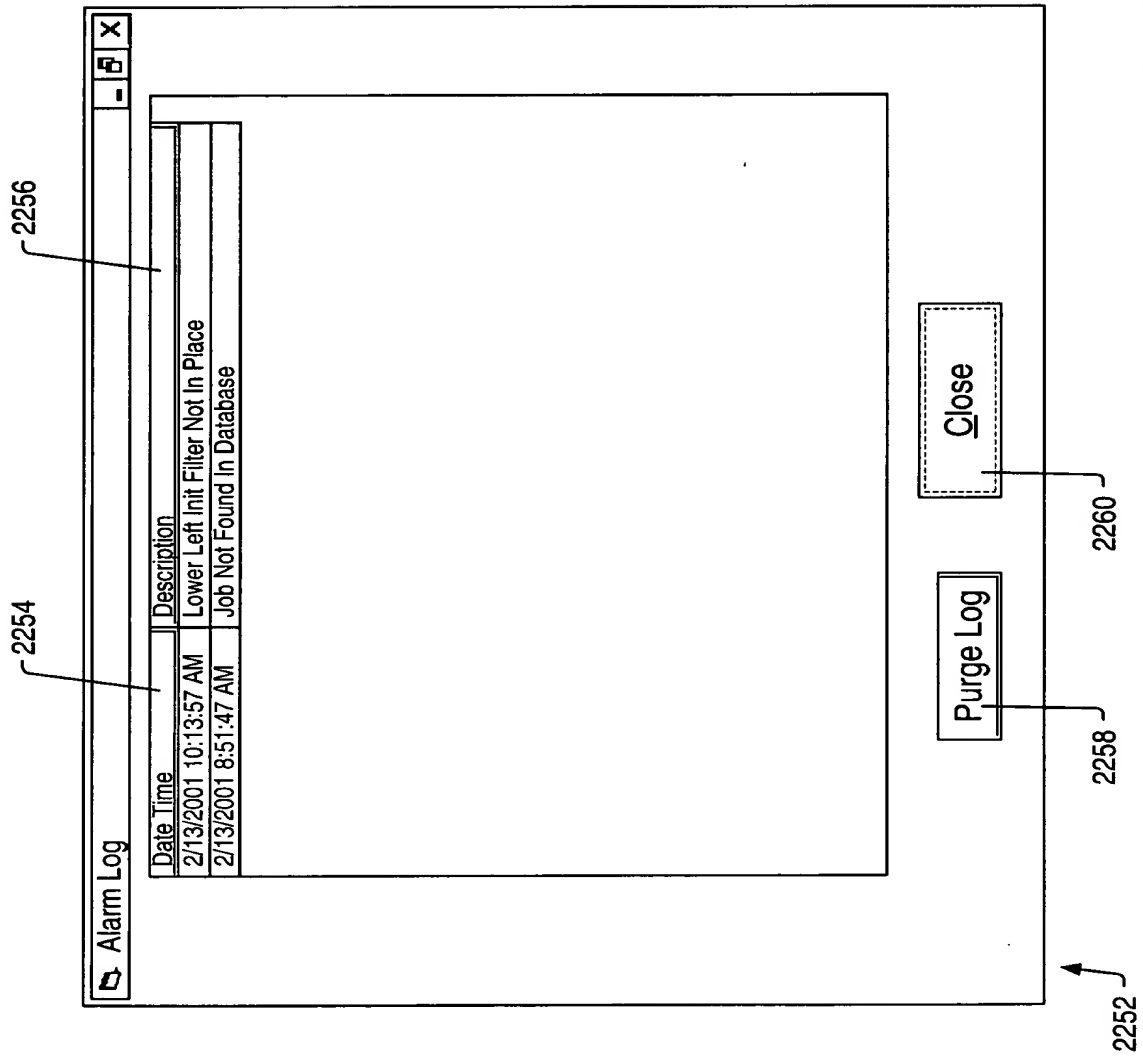


FIG. 49

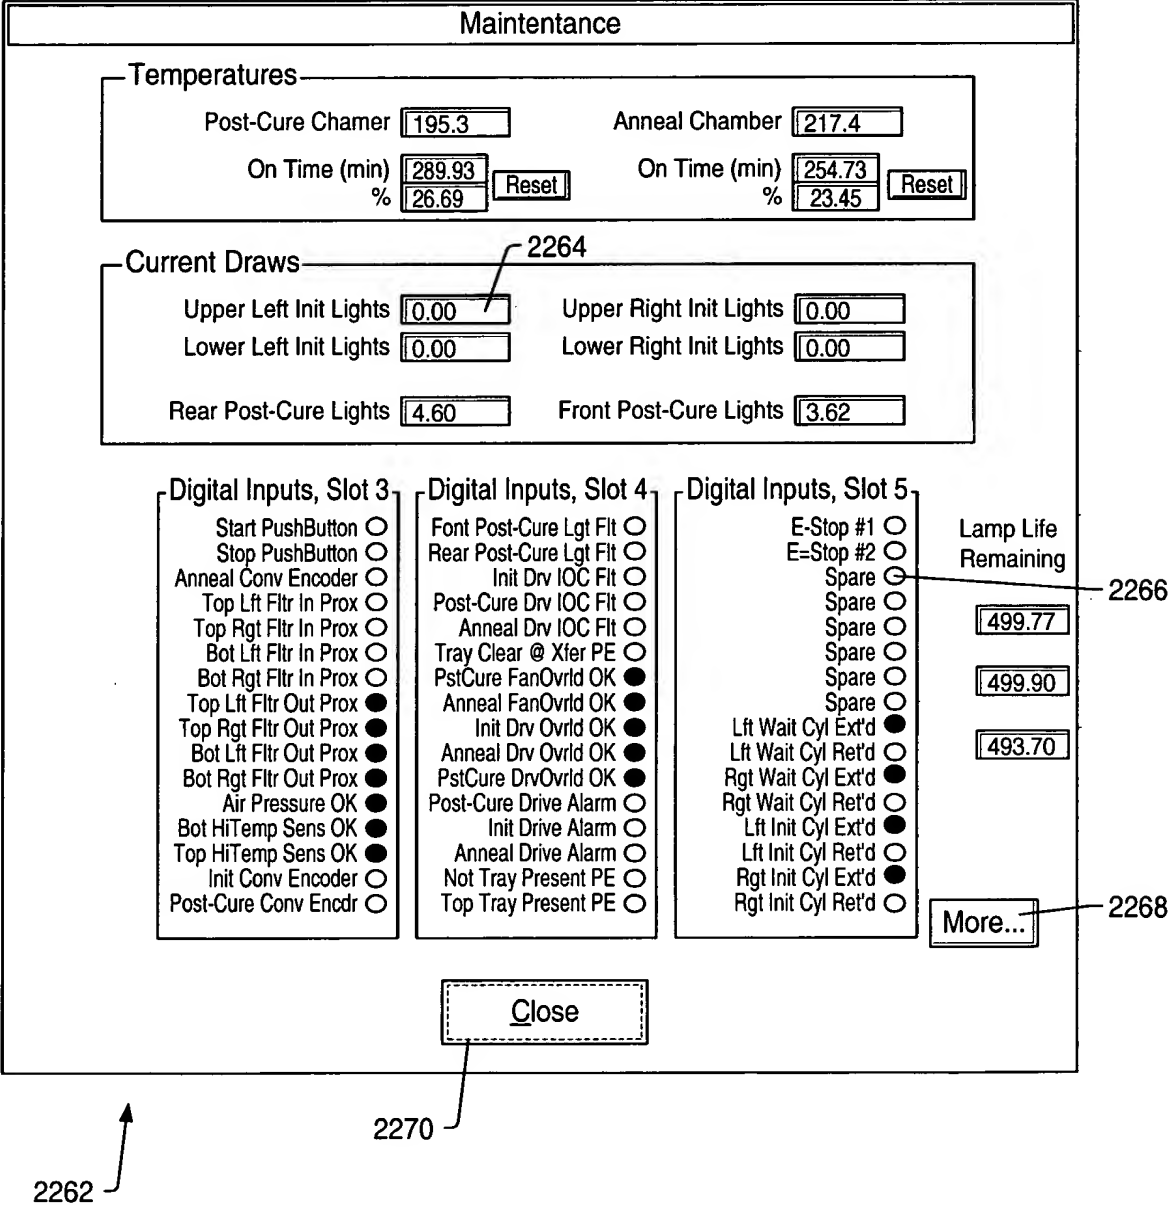


FIG. 50

Machine Setup

Anneal Conveyor

High Temp Alarm Limit
Temperature Setpoint
Low Temp Alarm Limit

Post-Cure Conveyor

High Temp Alarm Limit
Temperature Setpoint
Low Temp Alarm Limit

Initialization Lights

High Current Alarm Limit
Low Current Alarm Limit
No Scan Upper Init Time
No Scan Lower Init Time
No Scan Filter Select ☐

Post-Cure Lights

High Current Alarm Limit
Low Current Alarm Limit

Post-Cure Lights

Replaced Top Init Lamps ☐
Replaced Bot Init Lamps ☐
Replaced Post-Cure Lamps ☐

Save Changes **Cancel Changes**

2272 2278 2280 2274 2276

FIG. 51



Recipe DB

Job DB

Ticket Dir

Ticket Poll Rate (sec)

Ticket Print Scale (%)

Archive Jobs Every Days Keeping Days

v1.05

FIG. 52

2282

Job DB

Ticket Dir

FIG. 53

2296



3/44

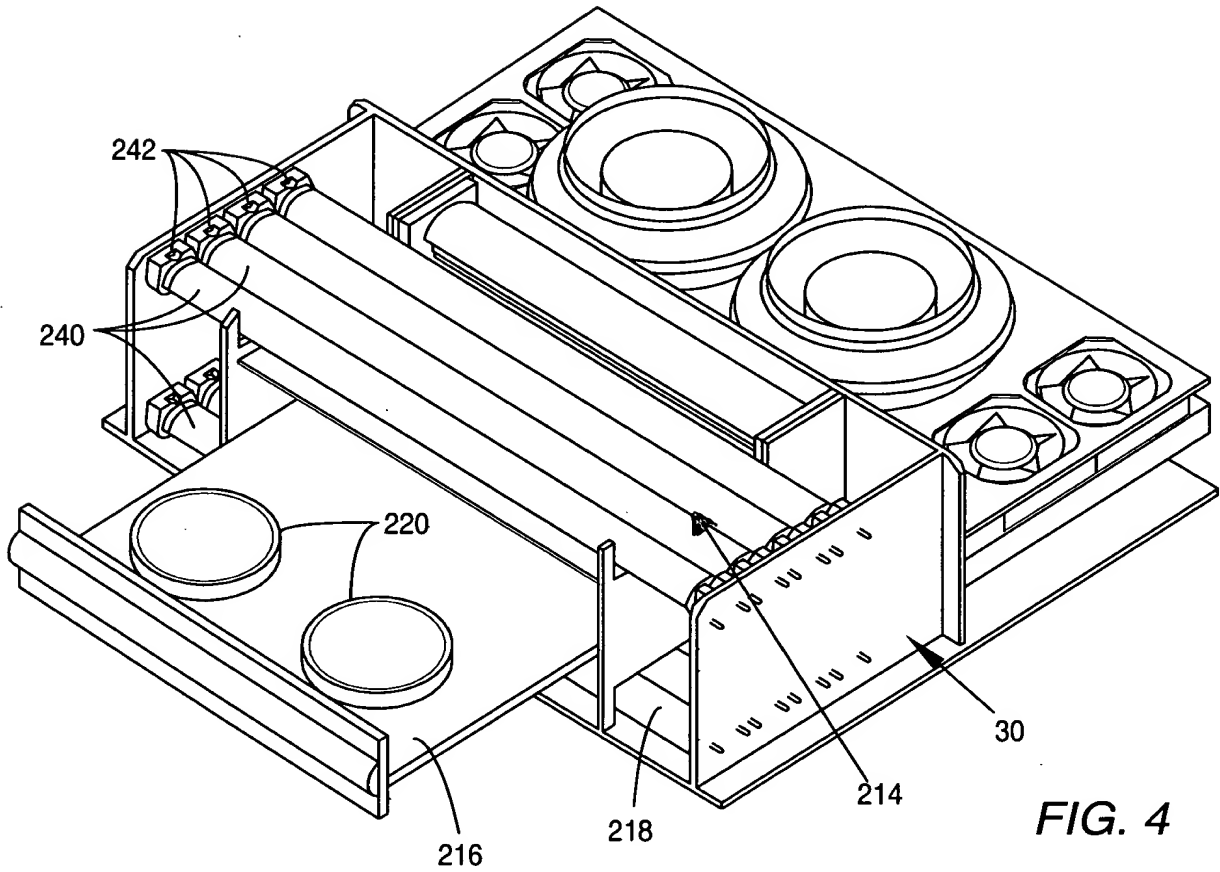


FIG. 4



15/44

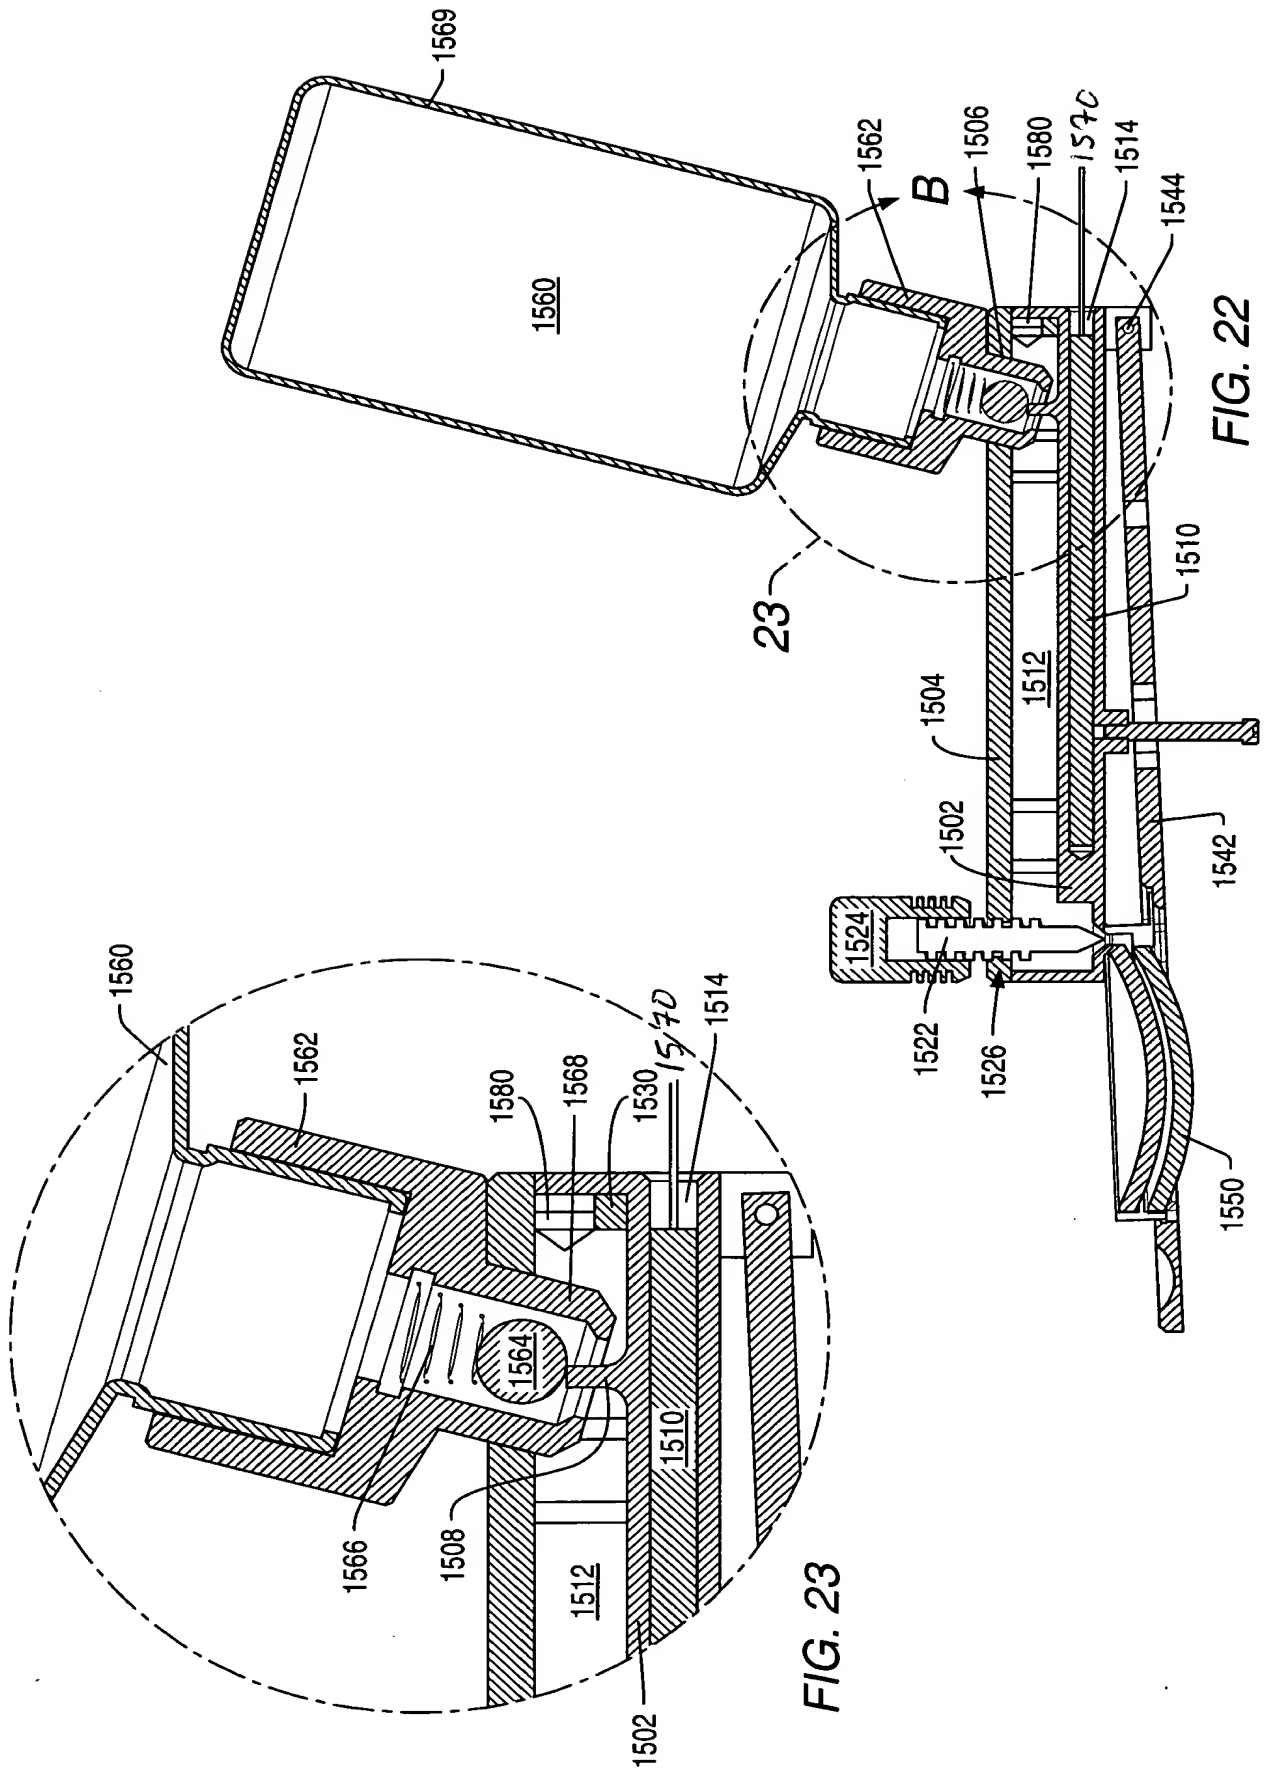


FIG. 23

FIG. 22



16/44

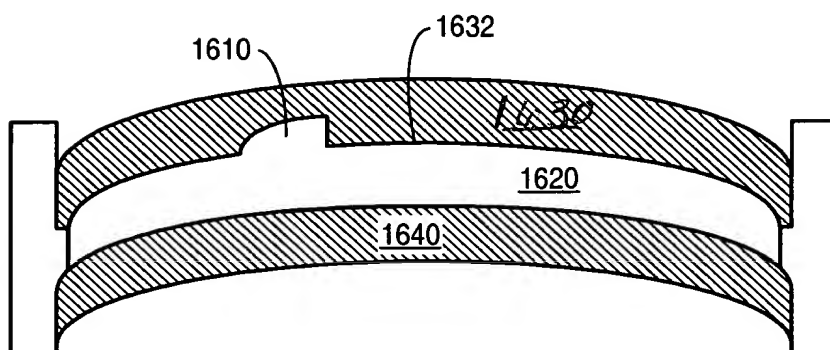


FIG. 24

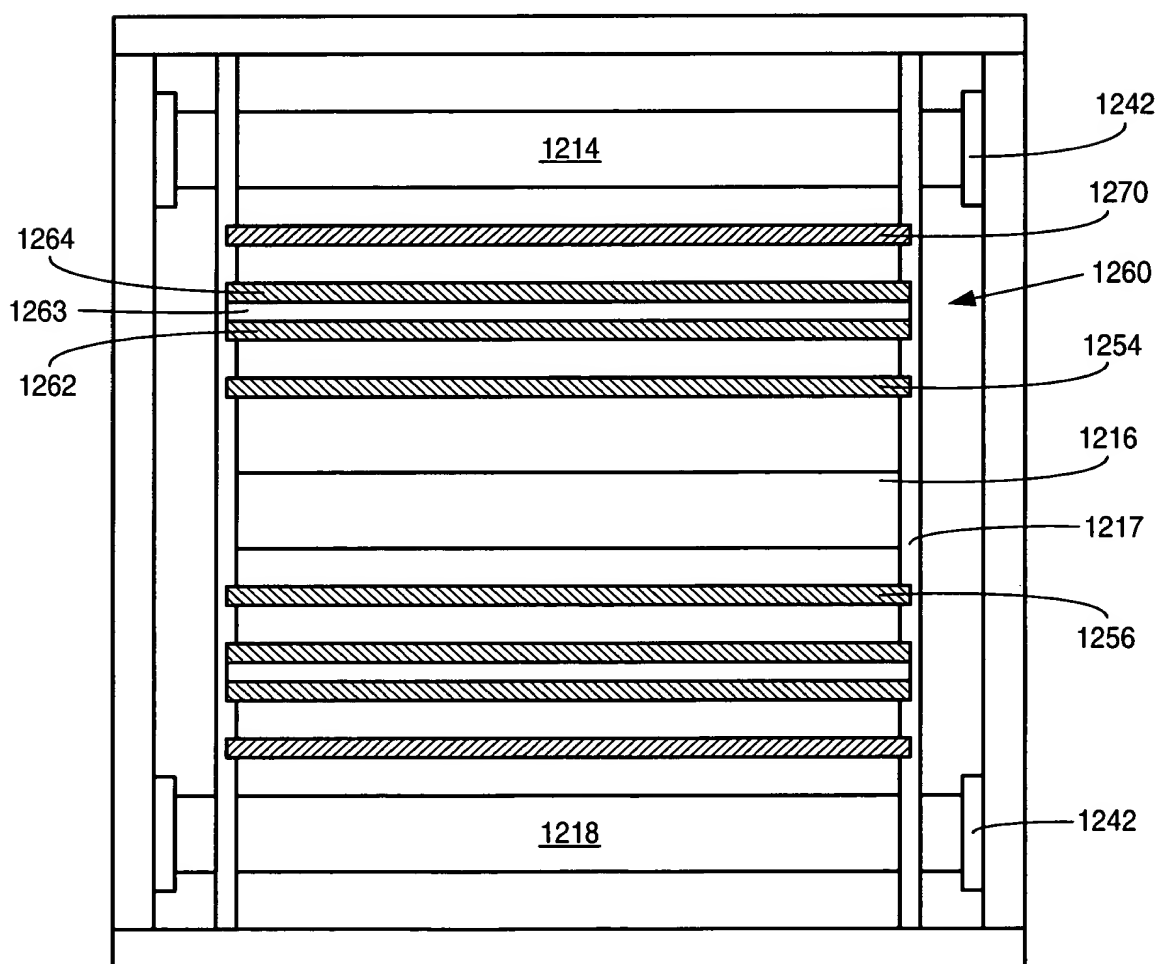


FIG. 25



22/44

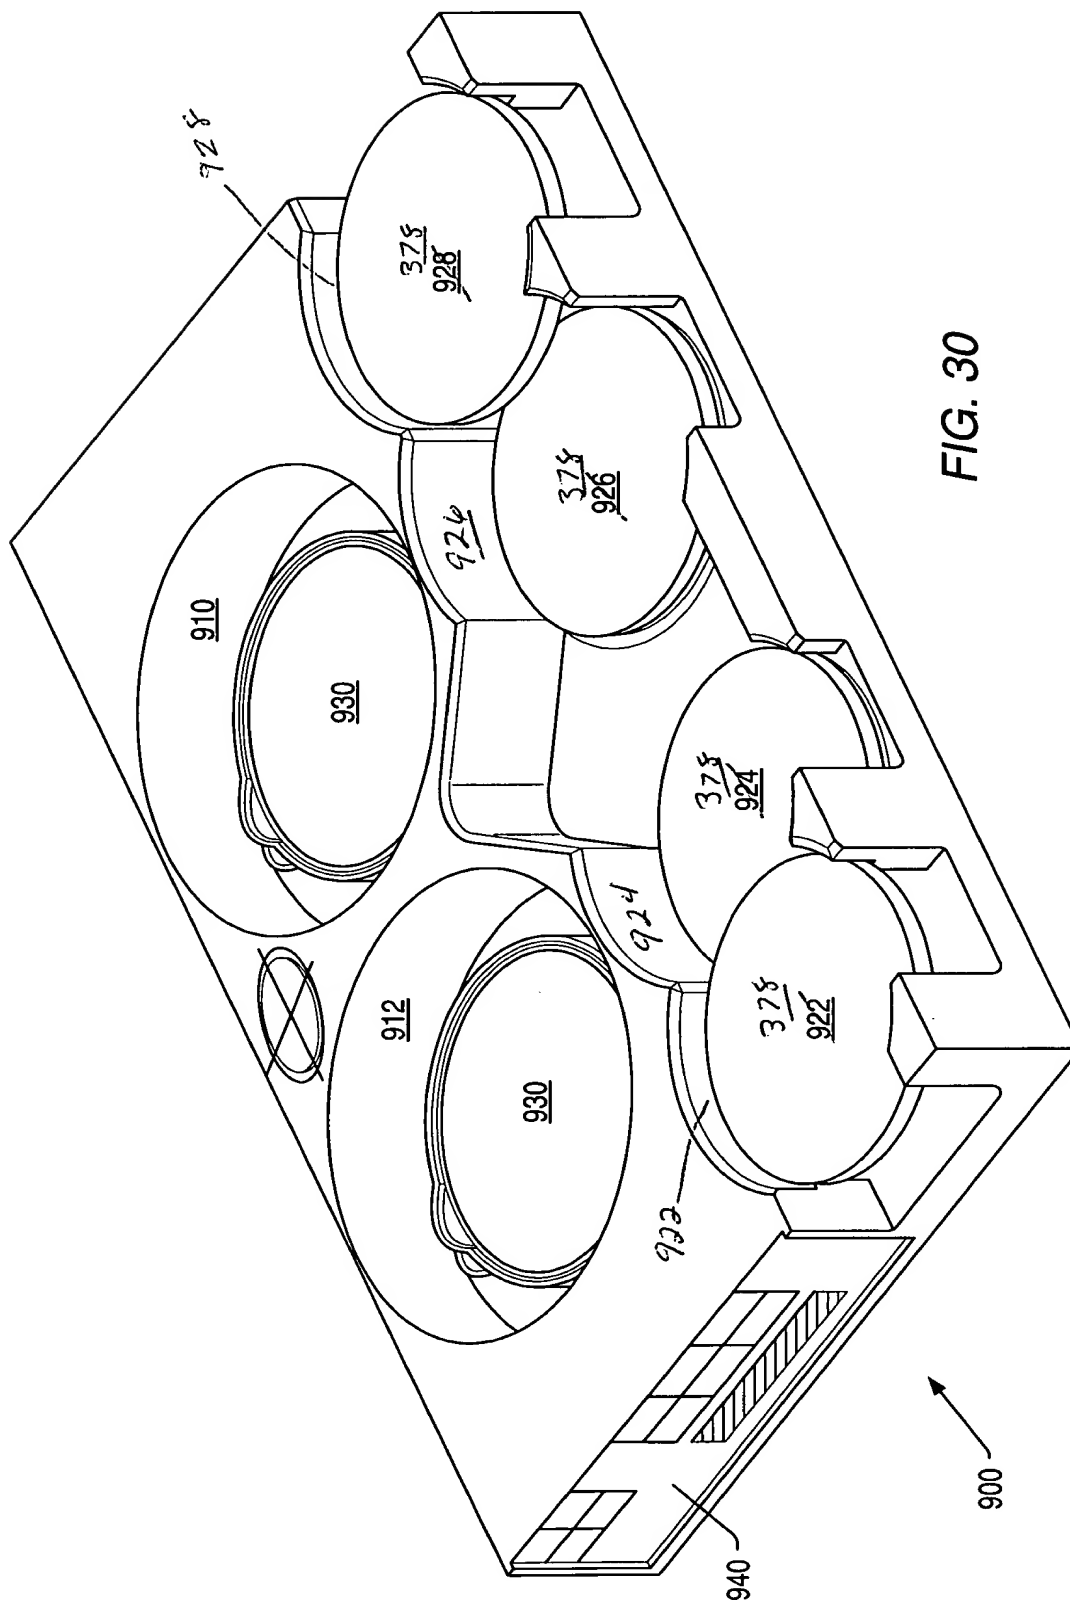


FIG. 30